

PVCuni and PVCduo

Process & Vacuum Controllers

- **UHV pressure measurement.** PVCuni 1 ion gauge. PVCduo 2 ion gauges.
- **2 secondary gauges.** Pirani, Intelligent 0-10 V gauges
- **Digital Interlock Hub.** User configurable seven trips and four digital inputs
- **Analogue Interfaces.** Two user-configurable analogue outputs
- **Multi-Step Bake-out controller.**
- **Timers.** Two user-configurable timers.
- **Full Computer Control.** MODBUS RTE and QueBUS (ASCII-based) protocols.

Table of Contents

1	SAFETY NOTES.....	4
2	Introduction	5
2.1	The PVCuni and PVCduo Controllers.....	5
2.2	Communications	5
2.3	Service and Repair	5
2.4	Declaration of Conformity.....	6
3	Specification.....	7
4	Installation and Setting Up	9
4.1	Physical	9
4.2	Controller Rear Panel	9
4.3	Controller Front Panel	9
4.4	Mains (Line) Voltage Selection and Fusing	10
4.5	Fuses	10
4.5.1	High Voltage Fuses	10
4.5.2	Internal fuses	11
4.5.3	Transformer Thermal Trips	11
4.6	Ion Gauge Cables.....	11
4.6.1	The 6 pin QM "power" connector	12
4.6.2	BNC Collector Connector	12
4.6.3	Ion Gauge Integrity, Safety and Fusing.....	12
4.7	Digital I/O Connector.....	13
4.7.1	Connector.....	13
4.7.2	Digital Trips	13
4.7.3	Digital Inputs	13
4.7.4	Weak +12V supply	13
4.8	Analogue Output Connector	13
4.9	Serial Communications.....	14
4.9.1	Overview	14
4.9.2	RJ45 Connectors	14
4.9.3	Daisy-chaining cable between controllers.....	14
4.9.4	USB and Ethernet Communications-based Hardware Kits	14
4.10	Data Retention (Volatile/Stored Parameters)	14
4.11	Factory Reset.....	14
5	Manual Operation	15
5.1	The Manual User Interface	15
5.2	Display Modes.....	16
5.3	Status Mode and Status Mode Pages.....	16
5.4	Menu mode	18
5.5	Parameter Mode: Button Operation and Parameter Data Entry.....	18
5.5.1	Parameter Types	18
5.5.2	Parameter States.....	18
5.5.3	Parameter Editing.....	19
5.6	Trips and Digital Input Status Indication	19

5.7	Communications Indication	20
5.8	Display Saver Mode	20
6	Ion Gauge Operation	20
6.1	Ion Gauge Construction	20
6.2	Ion Gauge and Relative Gas Sensitivity	21
6.3	Fixed Emission Currents and Auto-Emission	21
6.4	Emission Start-up, Filament Ramping and PID control	21
6.4.1	Emission Start-up	21
6.4.2	PID Emission Control	22
6.4.3	Start Power Learn Mode	22
6.5	Auto-Emission	22
6.6	Degas	22
6.7	Ion Gauge Status and Error Messages	22
6.8	PVCduo and Ion Gauge Emission Settings	23
6.9	Emission Leakage	23
6.10	Hints on using ion gauge measurements	23
6.10.1	Auto-Emission vs Fixed Emission	23
6.10.2	New Filaments – Conditioning and Degassing	23
6.10.3	Degas	23
6.10.4	The Ion Gauge Measurement Filtering	24
6.11	Ion Current and Beam Flux Measurements	24
6.11.1	Measurement Method	24
6.11.2	Measuring as Current	24
6.12	Ion Gauge Parameters	24
7	Secondary Gauging	26
7.1	Secondary Gauge Modules	26
7.1.1	Module Slots	26
7.1.2	Module Installation	26
7.2	Module Types	27
7.2.1	"E" Module: VSP52x Pirani Gauges	27
7.2.2	"F" Module: VSP84x Pirani Gauges	27
7.2.3	"W" Universal Module for Linearised gauges	27
7.3	Module Parameters	28
7.3.1	"W" Module Parameters	28
7.3.2	Module Calibration Parameters	28
8	Interlock Hub: Digital I/O and Analogue Outputs	28
8.1	Trips (Digital Outputs)	29
8.1.1	Relay-based Trips 1 to 4	29
8.1.2	Open Collector-based Trips 5 to 7	29
8.1.3	Trip Parameters	29
8.2	Digital Inputs	30
8.2.1	Digital Input Hardware	30
8.2.2	Digital Input Parameters	31
8.2.3	Digital Input Applications	31
8.3	Interlock Hub Status Page	31
8.4	Analogue Outputs	31

8.4.1	Overview	31
8.4.2	Analogue Output and Ion gauge Allocation	32
8.4.3	Digital Input Interlocking of Analogue Outputs	32
8.4.4	Analogue Output Parameters	32
9	Bake-out Control	33
9.1	Overview	33
9.2	Temperature Profile	33
9.3	Bake-out Interlocking	34
9.4	Display of Bake-out Operation	34
9.5	Bake-out Parameters	34
10	Dual (wide-range) Gauge Mode	35
10.1	Overview	35
10.2	DGM and Menu Parameters	36
10.3	Safe DGM Operation	36
10.4	Auto-cancellation of DGM Operation	37
11	Timers 1 and 2	37
11.1	Overview	37
11.2	Timer Interlocking	37
11.3	Timer Status Display	37
11.4	Timer Parameters	38
12	Calibration	39
12.1	Calibration	39
12.2	High Point (Gain) Calibration of Analogue Outputs	39
12.3	Low and High Dual Point Calibration	39
12.4	Calibration Menu Parameters	40
13	Setup Menu and Miscellaneous Parameters	40
13.1	Component Naming	40
13.2	Pressure Units	41
13.3	Menu and Display Related Parameters	41
13.4	Communications Parameters	41
13.5	Information Parameters	42

1 SAFETY NOTES



1. **This equipment MUST be earthed to a high integrity earth point.**
2. Voltages exceeding **400V** are present within the controller, and, during degas, on the cable and ion gauge head. Voltages up to **200V** are present on the cable and ion gauge head during normal (non-degas) operation. To prevent such voltages appearing between the chamber and controller, ensure that both are connected to a single, high-quality earthing (ground) point on the vacuum system using the screw terminal located on the rear panel.
3. **Before removing the top cover of the controller, allow at least 10 minutes for the high voltage capacitors to fully discharge. Unless technically qualified to do so, do NOT operate controller with the cover removed.** The top cover is connected to the base of the unit with a wire to ensure earth continuity. Do **not** remove this wire; ensure it is intact and tucked neatly between the transformer and side of the base before replacing the lid.
4. Always turn off power to the controller before connecting any cable or the ion gauge, or performing any maintenance to either.
5. It is the users' responsibility to ensure that the trips and digital inputs are employed safely. **In safety critical installations, an independent manual means of over-riding/inhibiting the trip signals is mandatory.**
6. Operation with the mains line voltage selector wrongly set voids warranty.
7. Careful design, commissioning and operation are essential to avoid damage to any part of the equipment configuration, or injury to personnel. In particular, consideration **must** be taken of the conditions and consequences of any part of the configuration failing, providing independent fail-safe mechanisms for protection, and ensuring that sensible safe limits are placed on controlled devices.

All conductors exposed to high voltage MUST be mechanically shielded to prevent contact with personnel.

Insulation MUST be rated at >500V continuous.

Where shielding involves metal, these parts MUST be connected to a high integrity earth.

In some situations, particularly at high pressures, dangerous high voltages can be coupled to any isolated metal parts of the vacuum system through the gas. This particularly relates to vacuum systems which use insulating components (e.g. glass, ceramic, plastic, rubber). All exposed and isolated metal parts should therefore be reliably grounded to a common system earth point via 4mm² or thicker copper wire/braid, the integrity of which should be checked regularly.

2 Introduction

2.1 The PVCuni and PVCduo Controllers

The new **Process & Vacuum Controllers** integrate the following functions in a single 1U high 19" rack-mounting unit:

- **UHV pressure measurement** to pressures below 1×10^{-12} mbar (gauge head dependent). The PVCuni supports 1 ion gauge head and the PVCduo 2 ion gauge heads operating simultaneously. Optionally, ion gauge measurements as current for beam flux applications.
- **Support for 2 secondary gauges.** The addition of modules provides support for a wide range of secondary gauges, including Pirani's and intelligent output gauges/controllers.
- **Wide-range gauge operation.** Ion and secondary gauges can be coupled to provide operation as of a single gauge head to provide atmosphere to UHV monitoring. Can provide auto pump-down functionality.
- **Digital Interlock Hub** comprising 7 trips (4 relays and 3 open-collectors) and 4 opto-isolated digital inputs. Fully user configurable to provide protection for the vacuum system, gauges and controller.
- **Analogue interfacing.** Two independent analogue outputs: user-configurable voltage range and pressure relationship.
- **Bake-out controller.** Built in K thermocouple input. Up to 6 ramp/soak steps with configurable gauge, digital I/O and user interlocking.
- **Timers.** Two independent user-configurable timers provide single shot or repetitive operations, such as pump conditioning, automatic timed valve operation, TSP switching..., with user defined interlocking.
- **Comprehensive communications.** All aspects of the controller are can be controlled via the RS232 and RS485 ports. Both the binary MODBUS RTE and the ASCII-based QueBUS protocols provide read AND write of MULTIPLE parameters within each comms exchange for fast throughput.

2.2 Communications

As indicated above, the controllers provide comprehensive serial communications capability. For further information, please refer to PVCUDSerialComms documentation downloadable from www.thyracont-vacuum.com, or contact direct@thyracont.de.

2.3 Service and Repair

The unit requires no maintenance. External dirt and soiling can be removed by a damp cloth. When returning the gauge for service please fill out a declaration of contamination and include it in the shipment. This document is mandatory to protect our service staff.

Download: www.thyracont-vacuum.com/en/support/maintenance-and-repair/ .

Important notes for disposal (Thyracont WEEE Reg.No.: DE 79715790)

According to WEEE directive 2012/19/EU and ElektroG3, the national law regarding distribution, withdrawal and environmentally acceptable disposal of electric and electronic equipment, this product must not be dumped in normal unsorted waste. For withdrawal and free disposal of used appliances please contact your Thyracont service or return the product with a filled-in declaration of contamination. Alternatively you can dispose used appliances at officially set-up collecting points.



The symbol of a crossed dustbin denotes that marked products must not be dumped in normal unsorted waste, but must be returned at officially set-up collecting points.

2.4 Declaration of Conformity



EU Konformitätserklärung *EU Declaration of Conformity*

Adresse / Address: Thyracont Vacuum Instruments GmbH
Max-Emanuel-Straße 10
94036 Passau
Germany

Produkt: Ion/Pirani Gauge Controller
Product: *Ion/Pirani Gauge Controller*

Typ / Type: PVCUxxx, PVCDxxx

Die Produkte entsprechen den Anforderungen folgender Richtlinien:
Product is in conformity with the requirements of the following directives:

2014/30/EU	Electromagnetic Compatibility (EMC)
2014/35/EU	Low Voltage Directive
2011/65/EU	EC directive on RoHS

Zur Überprüfung der Konformität wurden dabei folgende Normen herangezogen:
The conformity was checked in accordance with the following harmonised EN-standards:

EN 61326-1:2013 Group 1 / Class B
EN 61010-1: 2010
EN 50581:2012

Passau, 04.01.2021

Frank P. Salzberger, Geschäftsführer

3 Specification

Parameter	PVC <i>uni</i>	PVC <i>duo</i>
ION GAUGES:		
Number:	1 x UHV, dual Iridium-based filament. Yttria or Thoria-coated filaments.	2 x UHV, dual Iridium-based filament. Yttria or Thoria-coated filaments.
Filament Drive:	Electrically silent, high stability constant current dc.	
Gauge potentials:	Normal operation: Filament 40V. Grid: 200V. Degas: Filament 40V. Grid 400V+.	
Filament Drive:	0-3.5A (8V compliance) [PVC <i>duo</i> : per channel]	
Emission Control:	PID control with emission measurement for accurate pressure correction	
Manual Emission:	OFF, 0.06, 0.1, 0.15, 0.25, 0.4, 0.6, 1, 1.5, 2.5, 4, 6, 10mA	
Auto-emission:	Emission automatically optimizes to the measured pressure	
Start-up features:	Slow, standard and fast start-up. "Learn" feature for start-up power.	
Degas Type:	Thermal/Electron bombardment	
Degas: (Note 1)	2 stage: Ramp/Soak. Ramp: 1 to 499mins, to selectable level: low(15mA)/mid(25mA)/high(50mA), Soak: 1 to 499mins.	
Degas interlocking:	Pressure and digital input interlocking	
Degas Pressure:	Displayed during degas	
Degas on/off:	No interruption of ion gauge operation during degas start/stop transitions	
Electrometer:	Range: <1pA to 1mA. High stability, temperature controlled enclosure. [Allow ~40mins from powering up to stabilize.]	
Gauge Sensitivity:	1.0 to 99.9 (resolution 0.1)	
Gas Sensitivity:	0.01 to 99.99 (relative to Nitrogen = 1.00)	
Interlocking:	Digital inputs: trip/control operation/degas of the gauge.	
SECONDARY GAUGES:		
Number:	2 slots allow user to add support for secondary gauges by plug in modules. Any combination of "E" (for VSP52x Pirani), "F" (for VSP84x Piranis), "W" universal (user-configurable support of a range of intelligent gauges, external controller outputs) – see section 26.	
Module operations:	Module channels can operate in the same way as ion gauge channels, having interlock trips, digital inputs and analogue outputs assigned. They can be coupled with ion gauge channels for "dual gauge mode" operation.	
DUAL GAUGE MODE:		
Operation:	An ion gauge can be assigned a secondary gauge such as the combination act as single wide range gauge, with auto switching of on gauge operation	
BAKE-OUT CONTROL:		
Thermocouple:	Type K thermocouple built-in. 1 to 999°C (0.1°C resolution). Controls zone 1 bake-out.	
Bake-out Control:	User configurable: up to 6 ramp/soak steps, 0 to 99:59hm per step (1 minute resolution). Separate zone 1 and zone 2 temperature profiles	
Control Type:	On/off control. 1 second cycle time. User-defined temperature hysteresis.	
Power Control:	Any combination of the 7 trips can be assigned to switch heater power.	
Interlocking:	Each zone has independent ion gauge (separate ig 1 and ig2 for PVC <i>duo</i>), digital input and user interaction interlocks. Interlocks can independently <i>inhibit</i> heat output, <i>suspend</i> bake-out (inhibits output and stops bake-out clock, or <i>terminate</i> the bake-out.	
Parameters:	As well as setpoint, measured value and interlock information, peak temperature data available	
Ion gauge options:	Optional auto-degas of ion gauge(s) at end of bake-out	
DIGITAL INTERLOCK HUB:		


Number:	7 output trips and 4 digital inputs. Fully user configurable
Trips:	Trips 1 to 4: Single pole, change over relays rated at 1A@24Vdc/ 0.5A@40Vac Trips 5 to 7: NPN open collector, earth-referenced outputs. Max drive: 200mA and 12Vdc
Trip assignment:	Each trip is individually assignable to various ion/secondary gauge functions, bake-out, timers, front panel or external (comms) control etc.
Trip Options:	Operate/inhibit/override. Power up operation. Direction (< or > assigned parameter value). Operating hysteresis.
Digital Inputs:	All opto-isolated. 3- 5Vdc input. 2.4k Ω input resistance in series with LED. Reverse diode protected. Digital inputs 1 and 2: electrically isolated from each other and ground Digital inputs 3 and 4: electrically isolated from ground. Share negative input terminal.
Digital Input assignment:	Each digital input can be used as required for ion/secondary gauge protection/control, and interlocking of bake-out, timer
Digital Input options:	Invert input. Operate/inhibit/override. Power up operation.
Connector:	Standard DB25 connector.
ANALOGUE OUTPUT INTERLOCK HUB:	
Number	2
Output:	Full scale range: 0V to ~10.5V (12 bit resolution). Use calibration of max output.
Linearity:	$\pm 0.2\%$.
Assignment:	User configurable: Ion gauge (emission and sensitivity corrected), any secondary gauge, dual gauge, bake-out temperature...
Functionality:	User-defined voltage range, assigned pressure/temperature range, lin or log relationship...
TIMERS:	
Number:	2
Time Limits:	1 second to 999:59:59hms Cycle time defines off + on time
Operation:	Time can be set to start at start time, on time or user-defined time
Output Allocation:	Any combination of digital trips
Interlocking:	Digital input and ion gauge(s) inhibit of the output.
GENERAL:	
Dimensions:	19" rack mounting: WxHxD: 484x44x260mm (19"x1.73"x10.25") Allow 50mm (2") at rear for earth stud and connectors
Weight:	5.6kg
Electrical:	115/230Vac. 8W (gauges off), Max: 60W (full degas)
Protection:	Mains input: Both Neutral and Live fuse protected. 2A(T) for 230Vac; 3.15A(T) for 115Vac. Transformer: thermal trip protection
Display Type:	Graphic 200x16 pixel OLED display High brightness. High contrast. Long life >100,000h to half-brightness
Manual input:	Intuitive menu-driven via 5 front panel touch buttons
Communications:	Multi-drop RS232 (up to 8 units (port dependent)) and RS485-3 wire (up to 16 units). MODBUS protocol. Simultaneous multiple parameter read/write; floating point resolution. QueBUS protocol. ASCII-based protocol with multiple parameter read/write.
Communications connectors:	2x RJ45 for simple daisy-chaining

Note 1: PVCduo: Maximum total emission current (IG1 + IG2) is 56mA. An existing emission current takes precedence; the second gauge emission will be pinned to prevent a rise in total emission current above 56mA.

4 Installation and Setting Up

This section discusses controller installation, environmental issues, and the basics of instrument operation

4.1 Physical

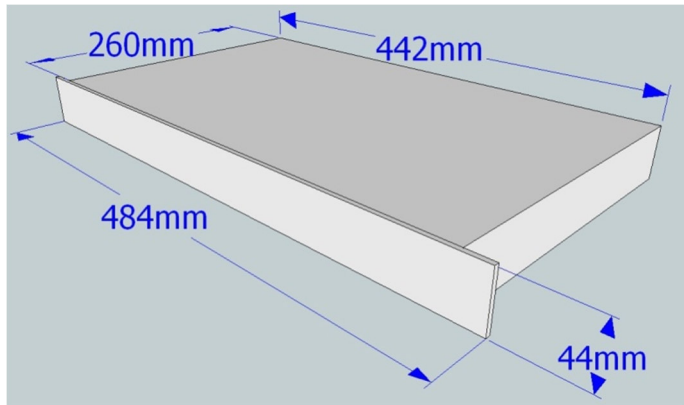

- The controller is enclosed in an earthed, metal, 1U high 19" rack-mounting enclosure.
- Please leave at least 50mm at the rear to accommodate the connectors and provide adequate ventilation for the fan
- The instrument should be mounted in a 19" rack, supported by runners/brackets beneath both sides; **do NOT support only via the front panel locating holes** as damage thus caused is NOT covered by warranty.
- Locate away from heat sources or cooling fans, at ambient temperature between 5 and 40°C.
- For ventilation, a 1U blanked gap is recommended between each group of 3 controllers.
- Avoid positioning near to equipment that generates high energy discharges. An ion gauge head located near a source of electrons or ions should be surrounded by an earthed fine-meshed screen to avoid disruption to operation.


Use of high frequency spark coils for leak testing should be avoided.

4.2 Controller Rear Panel



The upper controller is the PVCduo; the lower controller is the PVCuni.

4.3 Controller Front Panel

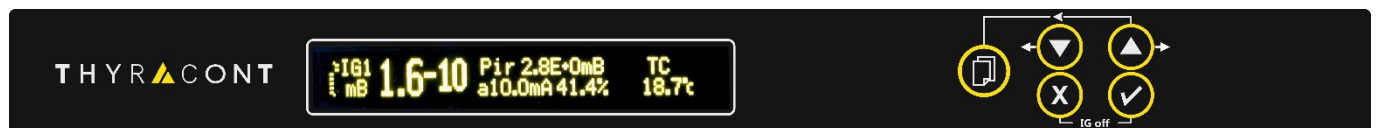


The picture shows one of many ways in which the values of the gauges and thermocouple are displayed for both the PVCuni and PVCduo. For more information, please refer section 15.

The 5 tactile push buttons are used for manual operation of the controller (section 15).

4.4 Mains (Line) Voltage Selection and Fusing

Mains power is connected via a high quality power filter, integrated with mains selection switch and fusing. To select line voltage and/or replace fuses:

1. Disconnect the mains plug.
2. Using a small flat-bladed screw driver, raise the hinged panel cover.
3. Using a small flat-bladed screw driver **placed at the long side of the red fuse holder (NOT the short sides)**, *gently* ease the voltage selector/fuse holder and remove
4. Both Live and neutral are fused. The holder accommodates either 5x20mm or ¼x1¼" fuses; the former fit into the rear section of the fuse slots. **For 230V use T2.0A; for 115V use T3.15A fuses. Slow Blow (type T) fuses.**
5. Replace the voltage selector/fuse holder **so that the required voltage shows through the window of the hinged panel cover.**

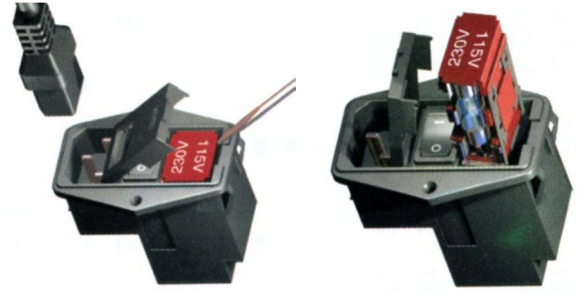

4.5 Fuses

As well the mains fuses, the controller has other protection devices.

4.5.1 High Voltage Fuses

The high voltage (grid) pin for the ion gauge connector is protected with a 100mA(F) **fast** fuse. This protects both the gauge head and the controller from short-circuits of the high voltage line.

This fuse is accessible from the rear panel and is marked "100mA(F)"; the PVCuni has one fuse, the PVCduo has two (one per ion gauge).

The fuse is housed in a bayonet type holder. To release the fuse:

- Turn the controller off and disconnect the power lead.
- Using finger or thumb, push the assembly in against the spring action - it will move by about 2mm
- Whilst pushing, twist anti-clockwise by about 60°.
- The fuse assembly will then be free to remove.
- **DO NOT APPLY FORCE AS THIS WILL DAMAGE THE FUSE HOLDER.**

To check a fuse, use a meter - blown fuses may visually look intact!

To insert a fuse:

- Insert the fuse assembly in the holder - there is only one position in which the fuse can be inserted all the way.
- Using finger or thumb, push the assembly in against the spring action.
- Whilst pushing, twist clockwise by about 60° to lock the fuse in place.

IF REPLACING THESE HIGH VOLTAGE FUSES, USE 100mA FAST FUSES. DO NOT USE TYPE 'T' FUSES AS THIS VOIDS THE PROTECTION OFFERED BY THE FUSE.

4.5.2 Internal fuses

As well as the high voltage fuses described in section 10, the controller has several internal fuses:

- The PVCuni has 3 internal fuses: 2x high voltage input fuses and 1x filament fuse
- The PVCduo has 4 internal fuses: 2x high voltage input fuses and 2x filament fuses (one per ion gauge).


It is unlikely that these fuses will need to be replaced as the current drawn through them is electronically limited. They are included in the event of a serious fault occurring, for safety and for fault diagnostics. If they need to be inspected or changed, please consult a qualified electrician or electronics engineer as high voltages may be present on these parts.

The photograph (right) shows the positions of the fuses in the PVCduo; the PVCuni lacks the second ion gauge filament fuse. To gain access to the controller, remove the 6 off M3 screws securing the lid (3 on each side). Lift the lid carefully, mindful of the earthing wire connecting it to the base; the wire is long enough to lay fold the lid and lay it to the side of the controller on its top.

As indicated on the PCB legends:

- The high voltage power supply input fuses are 250mA(T) (T = time-delay or slow-blow).
 - The filament fuses are 4A(F) (F = fast).
- DO NOT REPLACE THESE FUSES WITH VALUES AND TYPES OTHER THAN THOSE SPECIFIED.**

The fuses are protected by plastic covers - ALWAYS replace the cover if removed. As the covers are see-through, the state of fuse may be apparent without the need for electrical checks.

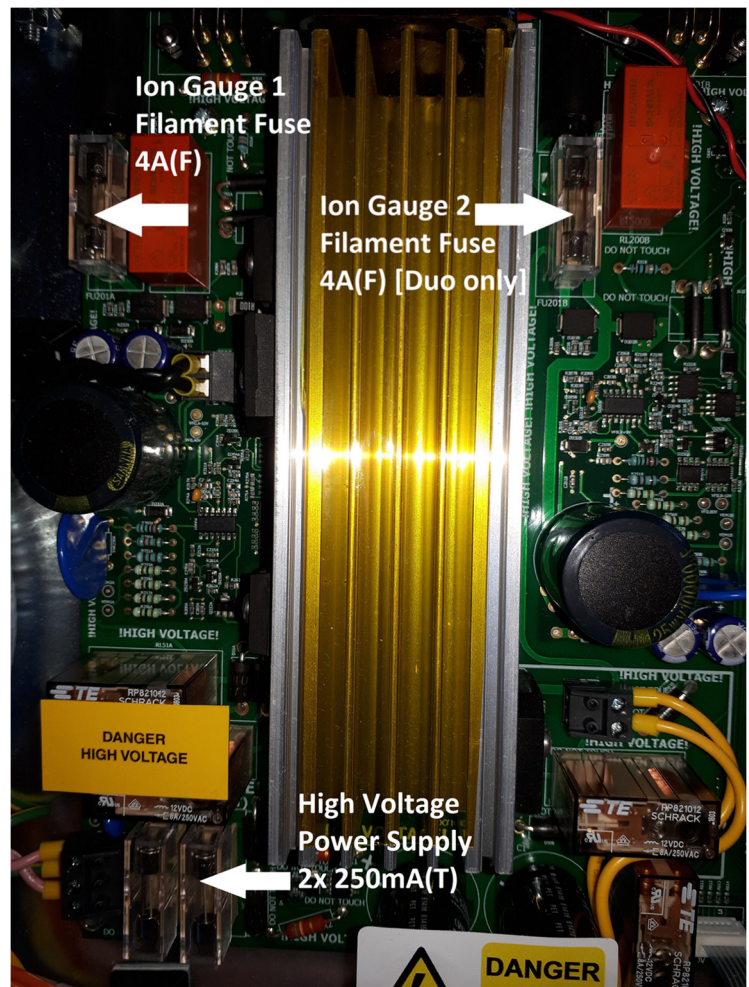

BEFORE ATTEMPTING TO CHECK THE FUSES, REMOVE ALL CONNECTORS FROM THE CONTROLLER (ESPECIALLY THE MAINS) AND ALLOW 10-15 MINUTES FOR THE HIGH VOLTAGES TO DISCHARGE FROM THE STORAGE CAPACITORS.

If any of these fuses is found to have failed, please consult the supplier of your controller for further information.

4.5.3 Transformer Thermal Trips

In addition to the fuses, the unit transformer contains thermal trips to protect against extended overload conditions. These are self-healing - they will reset when the transformer has cooled sufficiently.

4.6 Ion Gauge Cables

The ion gauge head is connected to the controller using 2 connectors: a 6 pin QM "power" connector, and a BNC connector for the collector current. **Potentially lethal voltages are present on the connectors; ALWAYS TURN THE CONTROLLER OFF BEFORE DISCONNECTING OR HANDLING THE CABLES.**

A high current capacity earth strap should be connected between the earth stud on the rear of the controller and the system's earth point.




Ion gauge cables bakeable to 200°C

Ready-made cable assemblies are available from your controller supplier.

4.6.1 The 6 pin QM "power" connector

Due to the high voltages present, only cables produced commercially or certified by qualified electrical engineers should be used. Accessories packs are available, which include parts needed to modify an existing cable for use with the controller.

Pin 1	Interlock (<i>Note 1</i>)
Pin 2	Grid
Pin 3	Interlock (<i>Note 1</i>)
Pin 4	Filament Common
Pin 5	Filament 1 (<i>Note 2</i>)
Pin 6	Filament 2 (<i>Note 2</i>)

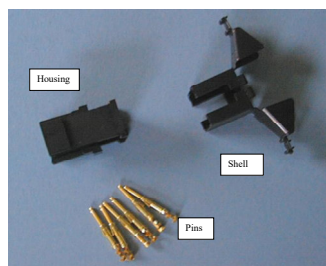

- Ion gauge connections to the 6 pin QM connector are as shown:
- Note 1:* Pins 1 and 3 **MUST** be linked either at the plug or the vacuum system as these indicate to the controller that a cable is connected. These act as a connection interlock
- Note 2:* Filament 1 and 2 allocation may vary between cable manufacturers. For single filament gauges, use either pins 5 or 6, and set the filament parameter appropriately.
- The ion gauges lead **MUST** conform to the following:
- CABLING **MUST** BE RATED AT THE **MAXIMUM** BAKEOUT TEMPERATURE
- Individual grid and filament wires **MUST** be rated at >5A AT THE MAXIMUM BAKEOUT TEMPERATURE
- The connection wires **MUST** be rated at >500Vdc

To modify an existing cable to connect to the controller:

Please check the function of each ion gauge cable wire before commencing as once the pins are inserted into the housing they are difficult to remove without special tooling.

- Remove the existing ion gauge connection connector
- Strip each of the wires ~12mm.
- Insert the bare wire into the pin; ensure the insulation is within the top crimp area of the pin.
- Crimp the bare wire section and top section to ensure an electrical connection that cannot be pulled out.
- Insert the pins into the housing from the rear. Ensure that each pin cannot be pulled out.
- If the existing ion gauge does not have interlock wires, connect a pin to each end of a 5cm long length of wire and insert to link positions 1 and 3.
- When all pins have been inserted, clip fit the shell onto the plug housing
- Secure the shell with the cable tie from the Accessories Pack as shown. This relieves strain on the individual conductors.

4.6.2 BNC Collector Connector

The small collector current is returned to the controller via a screened BNC connector, the central pin of which is connected to the collector, and the body to the earthed screen. Instructions on assembling BNCs are provided with the connectors, or can be viewed online.

To reduce the effects of noise picked-up on the collector lead, the controller provides analogue and digital input filtering. The default digital filter setting is 1 second. However, to ensure rapid response to pressure bursts (and thus good process reaction), the digital filter is disabled if a sudden large change in collector current is detected.

4.6.3 Ion Gauge Integrity, Safety and Fusing

- When the ion gauge is off, the high voltage grid and filament supplies are internally disconnected from the QM connector. However, before attempting any work on the ion gauge leads, disconnect the lead from both the controller and the ion gauge head.
- Pins 1 and 3 provide an interlock to detect the presence of the ion gauge. Ideally, these should be bridged *in vacuo*. However, if the gauge head does not have this facility, link the pins in the QM connector.
- When the ion gauge is on, the controller checks for gauge filament integrity and short-circuits between pins and to earth.
- The filament supply is based around a constant current source with a current limit of ~3.5A. The controller has a 4A fast fuse to protect the filament and controller from spurious fault conditions.
- High voltage to the grid and filament bias is protected via a 100mA(F) fast blow fuse. **DO NOT USE A "SLOW BLOW", "TIME DELAY" or "MAINS-STYLE" fuse in this position.**
- The controller has an internal PCB mounted high voltage 250mA (T) fuse.

4.7 Digital I/O Connector

4.7.1 Connector

A standard male DB25 connector provides access to the digital inputs and outputs.

4.7.2 Digital Trips

- **Trips 1 to 4** are change-over relays: **Do NOT exceed 1Adc or 0.5Aac at 32V**
- **Trips 5 to 7** are open-collector (Darlington pair) outputs with the emitter at 0V (earth potential) at pins 7 and 10. **Do NOT apply more than 14V (absolute maximum) or exceed MAXIMUM current for trips outputs 5 to 7 of 200mA.**

4.7.3 Digital Inputs

- The terminals of the digital inputs are each isolated using opto-couplers in series with 2k4Ω resistors.
- The digital inputs are internally protected against reverse bias
- Digital inputs 1 and 2 are electrically isolated positive and negative terminals
- Digital inputs 3 and 4 share a negative terminal (pin 20)
- Minimum guaranteed digital input operating voltage is 3.6V.
- **Do NOT exceed 32Vdc input to the digital inputs. If higher voltage are to be applied, limit the input current to 10mA by using an external series resistor.**
- The Digital inputs can be switched using an external relay contact, a logic gate or using an open collector output.

4.7.4 Weak +12V supply

A weak 12V supply is provided at pin 11 of the connector which is capable of powering the 4 digital inputs, thus obviating the need for an external power supply if switching via a relay or open collector device. The weak supply is fed via a protection diode and a 820Ω resistor, restricting the output current capable of switching the digital inputs to about 10mA.

This weak 12V supply is earth referenced, i.e. to pin 23. Thus if, for example, switching via an external relay, connect the digital input -ve to pin 23 and route the weak 12V supply from pin 11 via the relay contact.

Function	Pin	Pin	Function
		1	Relay 1 Normally Open
Relay 1 Common	14		
		2	Relay 1 Normally Closed
Relay 2 Normally Open	15		
		3	Relay 2 Common
Relay 2 Normally Closed	16		
		4	Relay 3 Normally Open
Relay 3 Common	17		
		5	Relay 3 Normally Closed
Relay 4 Normally Open	18		
		6	Relay 4 Common
Relay 4 Normally Closed	19		
		7	Outputs 5 to 7 0V (Earth)
Digital Inputs 3 and 4 -ve	20		
		8	Open Collector Trip 5
Open Collector Trip 6	21		
		9	Open Collector Trip 7
Digital 3 input +ve	22		
		10	Digital 4 input +ve
Outputs 5 to 7 0V. At Earth	23		
		11	Weak +12V (see 13)
Digital 1 input +ve	24		
		12	Digital input 1 -ve
Digital 2 input +ve	25		
		13	Digital input 2 -ve

4.8 Analogue Output Connector

The analogue outputs share is a standard "stereo" 3 pin 3.5mm (1/8") jack socket. The central pin is the analogue 1 output, the next ring is analogue 2 and the outer is 0V (earth). Screened signal wire is recommended

4.9 Serial Communications

4.9.1 Overview


The controller provides multi-drop RS232 and RS485 (3 wire) communications ports as standard. Both are available at two parallel-wired RJ45 sockets (see right); this arrangement provides for convenient daisy chaining of controllers. Up to 16 controllers can be attached to an RS485 port. Due to a multi-drop implementation, up to 8 controllers can be connected to an RS232 port (this may vary between PC's). See the Communications Handbook for further details.

Pin	Function	Colours
1	RS232 0V (Earth)	Orange/White
2	RS232 receive	Orange
3	RS232 transmit	Green/White
4	RS485 0V return	Blue
5	RS485 0V return	Blue/White
6	RS485 0V return	Green
7	RS485 transmit A	Brown/White
8	RS485 transmit B	Brown
Shield	Earth	Screen

4.9.2 RJ45 Connectors

The shielded RJ45 8/8 connector pin assignment and allocation is shown, along with the colours often used in commercially available cables. Note that the RS485 0V at pins 4, 5 and 6 is connected to internal 0V (earth) via a 100Ω resistor to reduce the likelihood of earth loops when using the RS485 interface.

If using RS485 interface, ensure that NONE of the RS232 pins are connected. If using an RJ45 patch lead, please ensure that ALL un-used wires are insulated from each other.

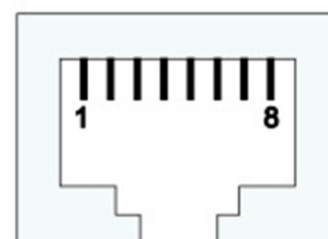

4.9.3 Daisy-chaining cable between controllers

The simplest method to daisy-chain controllers is to use standard RJ45 "patch" leads; shielded, Cat5 compliant cables are recommended.

4.9.4 USB and Ethernet Communications-based Hardware Kits

USB and Ethernet to serial port converters are readily available from many manufacturers. Often these contain multiple serial ports (2, 4, 8 or 16) and can be switched between serial port types (RS232, RS485, RS422).

4.10 Data Retention (Volatile/Stored Parameters)

The controller is operated by setting "parameters" either manually or over the communications interface. Some parameters are volatile, i.e. they are temporary and are not retained when the controller is powered off (for example, whether the ion gauge is on or off). Others are stored (in EEPROM). **Note: it may take up to 2 minutes before a changed parameter is stored in EEPROM; please allow this time if the controller is to be powered off.**

The controller loads the EEPROM data on power up. If a memory error is detected, a message is displayed (**Mem Error**) at the end of the power up sequence, and all parameter settings are reset to their default conditions.

4.11 Factory Reset

The parameters for the controller can be returned to their factory "default" values, i.e. the state in which the controller is shipped. To reset the controller:

- Turn the controller power OFF.
- Whilst simultaneously pushing and holding down the **CANCEL** and **ENTER** buttons, turn the controller power ON. [This is intentionally not easy to do to avoid accidental resetting the controller!]
- If successful, the message "Load Failed" appears briefly and the controller performs the parameter reset function.
- The controller then restarts itself, loading the default parameter values.

Note: The controller cannot be factory reset using a communications command.

5 Manual Operation






This section describes operation of the controller from the front panel

5.1 The Manual User Interface

The controller presents information via a 200x16 pixel OLED graphical display module.



The controller is controlled manually using 5 tactile buttons on the front panel .

			DOWN BUTTON Decrements Menu Level and Data Values		UP BUTTON Increments Menu level and Data Values
	MENU BUTTON Navigates Menu				
			CANCEL BUTTON Cancel Data Entry Exits Menu		ENTER BUTTON Enters new Data

Depending on context, the length of time certain buttons are held can change their function. For example, when in STATUS mode, pressing the **MENU** button will cause the controller to enter Menu mode displaying the title of the first menu; continuing to hold the button will scroll through the menu list.

The buttons are "membrane" types, comprising a domed area with a tactile response when pressed. They are designed to be used with fingers. **DAMAGE CAUSED BY USING SHARP OBJECTS ON THE BUTTONS IS NOT COVERED BY WARRANTY.**

NOTE: Pressing the CANCEL and ENTER buttons together at any time will turn off emission to ion gauge(s) immediately.

5.2 Display Modes

There are 4 “modes” of controller operation:

MODE	Description	Buttons
STATUS: (section 16)	Provides information about controller operation via a number of “pages”	DOWN : Move to next status page UP : Move to previous status page MENU : Enter MENU mode CANCEL : Changes the screen to show alternative data; for example,, output power instead of emission current in pages showing ion gauges whilst held down
MENU: (section 18)	Display is divided into two: left shows ion gauge status, right is the menu selection areas.	MENU : Move to next menu DOWN : Move to next menu UP : Move to previous menu MENU+UP : Move to previous menu-drive CANCEL : Return to Status mode (at last page displayed) ENTER : Enter the Parameter editing mode at the first parameter in the menu
PARAMETER: (section 18)	Display is divided into two: left shows ion gauge status, right is parameter selection and editing area.	MENU : Move to next parameter MENU+UP : Return to previous parameter UP : Increment the selection or increases the number at the cursor position DOWN : Decrements the selection or decreases the number at the cursor position CANCEL : If the parameter value has been modified, initially returns the parameter value to its current value. If held, returns to the Menu mode at the menu position ENTER : Sets the display value into the parameter
DISPLAY SAVER: (section 20)	Display shows minimum data relating to operating gauges. Data scrolls slowly across the display.	Starts if no buttons are pressed for longer than the Display Saver Time parameter Pressing ANY BUTTON returns the display to the last status page being viewed

5.3 Status Mode and Status Mode Pages

The controller conveys information via the Status mode pages; each page relates to a specific feature of the controller. In the Status mode, you navigate the pages using the **UP** and **DOWN** buttons. Note that some of the pages for the PVCduo are missing for the PVCuni.

The following table summarises the pages, in order, and their function. Examples of page displays are provided in subsequent sections:

PAGE (Index)	Notes	Description	Graphic/Text	uni/duo
General (0)	1,2,3	Data from ion gauge(s), thermocouple input and modules (if fitted) displayed as 2 lines of 34 text characters.	T	ud
IonGauge1 (1)	1,3	Displays ion gauge 1 data in large font. Secondary gauges (if installed) and thermocouple scrolled	GT	ud
IonGauge2 (2)	1,3	Displays ion gauge 2 data in large font. Secondary gauges (if installed) and thermocouple scrolled	GT	Duo only
Ion Gauge 1 and 2 (3)	1,2,3	Displays both ion gauges in large font. Secondary gauges (if installed) and thermocouple scrolled	GT	Duo only
BarGraph (4)	1,2,3	Upper screen: Ion gauge(s) (in dual gauge mode if enabled) displayed as bar graphs . Lower screen: All gauges data scrolled and displayed as text.	GT	ud
Modules (5)	1,3	Displays data from both modules as large font. Thermocouple and ion gauge(s) data (if operating) scrolled	GT	ud

Bake-out (6)	4	Provides summary of currently operating bake-out, or termination condition of last bake-out executed. Press and hold CANCEL to show peak temperatures achieved in current (or previous) bake-out	T	ud
Interlock Hub (7)	5	Summarizes the current states of the 7 trips (top line) and 4 digital inputs (bottom line). Press and hold CANCEL to show scroll through the 7 trips showing their status and current allocation	T	ud
Timers (8)	6	Summarizes the status of the 2 timers	T	ud

Note 1: Ion gauge values: press and hold **CANCEL** to show output power instead of emission current

Note 2: Secondary gauge and thermocouple data scrolled

Note 3: Pressing **MENU** starts menu access at ion gauge 1 menu

Note 4: Pressing **MENU** starts menu access at bake-out menu. Pressing **CANCEL** provides peak temperatures attained

Note 5: Pressing **MENU** starts menu access at trips menu. Pressing **CANCEL** provides summary of DIO settings

Note 6: Pressing **MENU** starts menu access at timer 1 menu. Pressing **CANCEL** provides summary of timer settings

Examples:

PVCuni Bargraph Page

PVCduo Bargraph Page. The ion gauge(s) toggle between IG1 and IG2

Ion Gauge 1 Page. Pressure Display with secondary devices

Ion Gauge 1 Page. Pressure Display with emission details

5.4 Menu mode

From the Status Mode, pressing the **MENU** button to enter Menu mode. The order of menus is:

Ion Gauge 1 Menu
Ion Gauge 2 Menu^{Note 1}
Module 1 Menu^{Note 2}
Module 2 Menu^{Note 3}
Trip 1, 2, 3, 4, 5, 6 and 7 Menus
Digital Input 1, 2, 3 and 4 Menus
Analogue Out 1 and 2 Menus
Bake-out Menu
Ion Gauge 1 Dual Gauge Menu
Ion Gauge 2 Dual Gauge Menu^{Note 1}
Timer 1 and 2 Menus
Calibration Menu
Setup Menu
 (returns to Ion Gauge 1 Menu)

Note 1: PVCduo only.

Note 2: Only if 'U' or 'W' module installed in Slot 1.

Note 3: Only if 'U' or 'W' module installed in Slot 2

Once in Menu mode:

- To move forward through the menu list, press either the **MENU** or **DOWN** buttons
- To move back through the menu list, press either the **UP** or the **MENU+UP** buttons together
- To leave menu and return to last status mode page, press **CANCEL**
- To enter the menu for parameter editing, press **ENTER**

Note that the first menu displayed on pressing **MENU** when in status mode depends on which page is being viewed:

- If viewing the Trips and Digital input summary page, menu mode is entered at Trip 1 menu
- If viewing the Bake-out page, menu mode is entered at Bake-out menu
- If viewing the Timer status page, menu mode is entered at Timer 1 menu
- For all other pages, menu mode is entered at Ion Gauge 1 Menu

5.5 Parameter Mode: Button Operation and Parameter Data Entry

5.5.1 Parameter Types

There are 3 parameter types:

- **SELECTION PARAMETERS:** These are parameters requiring selection from a limited range of options. Examples: ion gauge emission, allocation of trips, analogue outputs...
- **NUMERICAL DATA PARAMETERS:** These parameters require a numerical value. The controller takes care of formatting the parameter (integer, decimal, scientific, time) applying the relevant number of decimal places and restricting the input to the parameters range. Examples: Trip pressures, bake-out step times and temperatures...
- **TEXT PARAMETERS:** These parameter require entry of alphanumeric characters. Examples: unit and gauge names...

5.5.2 Parameter States

Parameters can be in 3 states:

- **LOCKED** parameters are indicated by a key symbol. The parameter cannot be edited. This may be because it is for information only (e.g. the heatsink temperature), the parameter would have no effect (e.g. the ion gauge emission if the gauge is disconnected at the rear panel), or the parameter is a "protected" type requiring parameter unlock being activated (e.g. calibration parameters).

Note the "key symbol" which indicates that the parameter is locked and cannot be edited.



- **CURRENT VALUE;** the equals sign ('=') indicates that the display shows the current value of the parameter and the parameter can be edited. In the example shown, this is because calibration had been unlocked (see section 39)



- **NEW VALUE**; the question mark '?' indicates that the display is showing a new parameter value. Note that the new value is not used until **ENTER** button is pressed, at which point the '?' changes to '=' indicating that this is the operating parameter value.

5.5.3 Parameter Editing

Data presentation and the method for changing their values depends on the type of parameter:

SELECTION PARAMETERS:

The example below shows changing the emission current. On entering the parameter, the middle image indicates that the emission is off. Pressing the **DOWN** button changes the option to Auto emission, and pressing the **UP** button to the minimum emission value (0.1mA). Note the '?' indicating the change to the value.

To exit without changing, press **CANCEL**. To enter a new value, press **ENTER**.

DATA PARAMETERS:

Data parameters require numerical data entry. In these cases, an underline cursor indicates the currently "active" digit:

- Briefly pressing and releasing (0.2 – 0.8 second) **DOWN** moves the cursor one character to the left
- Briefly pressing and releasing (0.2 – 0.8 second) **UP** moves the cursor one character to the right-hand
- Pressing and holding (>1 second) **DOWN** decreases the parameter value at the cursor position. Continuing to hold scrolls the value
- Pressing and holding (>1 second) **UP** increases the parameter value at the cursor position. Continuing to hold scrolls the value


Note: the new value is automatically checked against the range of the parameter, pinning the value to within the parameter range.

In the case of exponential data formats, the cursor appears below the entire exponent section. The **UP** and **DOWN** buttons increments/decrements the value over the entire exponent range.

TEXT PARAMETERS:

The unit, ion gauge and secondary gauge names are text parameters. These behave like data parameters, except the character range is not limited to numbers. Valid characters are: ' ' (space), '0' to '9', 'A' to 'Z' and 'a' to 'z'.

5.6 Trips and Digital Input Status Indication



The status of the 7 trips and 4 digital inputs are indicated at the far left of the display, regardless of display mode. The display toggles between displaying trip state and digital input state every 2 seconds.

DIGITAL INPUT INDICATION

The states of the 4 digital inputs are indicated by 4 bars, the topmost being digital input 1, the bottom one being digital input 4. The figure shows the 4 possible states: DI1 = OFF, DI2 = ON, DI3 = Inhibit, DI4 = Override.



TRIP INDICATION

The states of the 7 trips are indicated by 7 bars, the top most being trip 1, the bottom one being trip 7. For example, the figure indicates that trips 1, 2 and 3 are on, trip 4 is overridden, trips 5 and 6 are off and trip7 is inhibited.

5.7 Communications Indication

If the communications indicator is switched on (see section 41), the top left pixel of the screen will flash during communications. Note that as the display rate and communication arrival rates are not synchronized, the rate of flashing does not correspond directly to communications messaging rate; rather, it is purely an indicator of communications.

5.8 Display Saver Mode

At times when the controller is not going to be observed (e.g. over-night), the user can set the display to enter Display Saver Mode. If no buttons are then pressed for longer than the **Display Saver Time** parameter (see section 41), the display will only show information for operating devices on the controller. This information slowly scrolls across the screen:

IG 2.3e-10 Pir 2.2e-3

IG 1.7e-10mB TC 178.5°C 11:13hm

The displayed information comprises 2 fields:

- Ion Gauge(s): If an ion gauge is operating, the gauge name and pressure are indicated. For the PVCduo, if both gauges are operating, the information shown toggles between the two ion gauge values. If no ion gauge is operating, this field is blank
- Secondary Gauges/thermocouple: This field toggles through the 3 potentially operating secondary devices: Slot 1 module, Slot 2 module and thermocouple. If a slot is empty, it is ignored. The device name and its value are displayed, and, if a bake-out is occurring, that is followed by the remaining time.

The controller reverts to the last observed Status Mode page as soon as any button is pressed.


6 Ion Gauge Operation


The controller provides stable and electrically silent (dc) control of a UHV ion gauge head. This section discusses ion gauge operation and some of the features offered by the controller such as Auto Emission, Degas pressure measurement, new filament conditioning and uninterrupted normal/degas transitions.

6.1 Ion Gauge Construction

An ion gauge head comprises:

- A filament assembly, usually comprising 2 independent filaments biased at $\sim +45V$ wrt earth. The filaments are Iridium, coated with either Thorium or Yttrium to reduce the work-function for emission of electrons.
- A cylindrical grid biased at $\sim +190V$ during normal operation and $\sim +400V$ during degas that attracts the electrons. Its open structure ensures that electrons make multiple passes through it before being collected. Electrons that strike a gas molecule ionize it, and the resulting positive ion is attracted to...
- A thin "collector" wire in the middle of the grid. The tiny ion current is measured in the controller by a very sensitive electrometer.

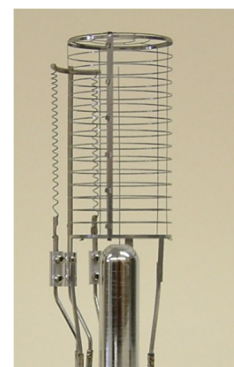

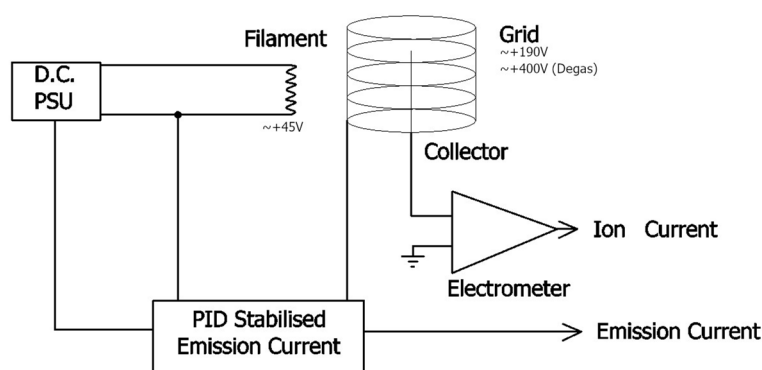

The measurement process is shown in the schematic. In the PVCs, the filament is heated by a high stability, low noise, constant current source. The emission current from the filament to the grid is PID stabilized at the desired value. The controller simultaneously measures the ion current **AND** the emission current to determine the pressure.

Because of the very large dynamic range of the ion current (10^{-12} to 10^{-2} Amps), emission currents are adjusted to match the pressure range of interest; for example, the Auto-emission setting automatically selects the optimum emission for the measured pressure.

The need to measure very low currents means that the electrometer amplifier is sensitive to thermal variation; a notable feature of the PVC design is the siting of the electrometer in a "thermal" oven that keeps it at a near constant temperature.

6.2 Ion Gauge and Relative Gas Sensitivity

The efficiency of ion generation depends on the design/geometry of the gauge head. The "Ion Gauge Sensitivity" parameter allows the accepted value for the ion gauge head to be input into the controller; values typically vary between 5 and 30 mbar⁻¹.

Ionization probability also differs with gas type. This sensitivity to gas species is referenced to Nitrogen (as 1.00); values for some gases are shown below, and these, too, can be entered as an ion gauge parameter.

The overall "gauge" sensitivity = (gauge sensitivity) x (relative gas sensitivity). Note that the relative sensitivity values also vary with gauge head design, and values even between "identical" gauges can vary by 10% or more. Relative sensitivity values become less reliable with increasing pressures above about 10^{-5} mBar.

H ₂ 0.46	Air/N ₂ 1.00	NO 1.15	CH ₄ 1.40
D ₂ 0.35	O ₂ 1.01	NH ₃ 1.22	C ₂ H ₆ 2.60
He 0.18	CO 1.05	Ar 1.29	C ₃ H ₈ 4.21
Ne 0.30	H ₂ O 1.12	CO ₂ 1.42	Kr 1.94
			Xe 2.86

6.3 Fixed Emission Currents and Auto-Emission

The controller provides a range of "fixed" emission currents: 0.06, 0.1, 0.15, 0.25, 0.4, 0.6, 1, 1.5, 2.5, 4, 6 and 10mA; note that each value is approximately 1.5x the previous value to provide an "exponential" sequence. Optimum choice of which emission to use depends on the operating pressure range of the vacuum system; higher emission currents are required at lower pressure to boost ion current. The controller also provides an "Auto-emission" setting that automatically adjusts the emission current to match the gauge head operating conditions (section 22).

The user can define a minimum and maximum emission setting to reflect optimum conditions for a specific design of ion gauge head, for example, to limit the maximum current (manual or auto-emission) to 4mA.

6.4 Emission Start-up, Filament Ramping and PID control

Ion gauge has 2 modes of operation: Start-up and Emission control.

6.4.1 Emission Start-up

The ion gauge emission is ramped up in 2 stages. Initially the power is ramped from zero power to the value specified by the **Start Power** parameter value. The rate at which the power is ramped can be selected using the **Filament Ramp Rate** parameter as slow (0.2% per second), standard (1% per second) or fast (10% per second). If, during this period, emission is established, emission control takes over.

If emission is not established by the time the **Start Power** parameter is reached, the second stage commences, ramping the power at a rate of 0.5% per second until emission is established. If emission fails to occur by the time power has reached 75% of the **Max Power** parameter value, emission for the filament is deemed to have failed.

6.4.2 PID Emission Control

Once emission is established, the μ processor employs a PID control loop to maintain emission stability at the required value. The **PropBand** and **Damp** parameters are set to 25 arbitrary units which is suitable for most ion gauge designs. During normal PID operation, the power level is maintained between the **Minimum Power** and the **Maximum Power** parameter values.

6.4.3 Start Power Learn Mode

For optimum start-up of an ion gauge (for example, when using fast ramp rate, or in DGM mode when switching from secondary to ion gauge), having a **Start Power** appropriate to the gauge is important. The **Filament Ramp Rate** parameter provides the **Learn Start Power** option. On ion gauge start-up, this forces the controller to perform a slow (0.2%/s) ramp until emission is established - the power value at which emission starts is automatically stored in the **Start Power** parameter for future use.

Note: The Learn Start Power option should NOT be used with a new filament or one that has not been adequately conditioned by use; conditioned filaments require less power than new ones - see section 23.

6.5 Auto-Emission

In "Auto-emission" the controller selects the most appropriate emission current (within the **Minimum** and **Maximum** emission range) for the measured pressure; the lower the pressure, the higher the selected emission.

To avoid pressure bursts, auto-emission ramps the emission; it ramps the emission more slowly when increasing than when decreasing. However, to protect the ion gauge, the Auto-Emission algorithm responds immediately to sudden increases in pressure.

6.6 Degas

After air exposure, or extended filament non-use *in vacuo*, starting an ion gauge can degrade the vacuum due to out-gassing, and can adsorption can influence operation of the collector; effectively these change the sensitivity of the gauge. A gauge can be "cleaned" by raising the emission current and grid potential above normal operating values, so-called "degassing". The frequency and extent of degassing depends on the process, but a long (>30 min) is generally recommended after air exposure (usually following bake-out).

The controller provides 3 levels of degas, Low, Mid and High, which set the emission current to 15, 25 and 50mA respectively; the grid potential is also raised to ~400V to enhance grid heating. The high emission currents also drive the filament at a higher power (thus temperature).

Degas is a 2 step process. Emission is ramped from the current emission to the selected degas level and then held. The duration of the **Degas Ramp** and **Degas Hold** parameters can each be 1 to 499 minutes.

The controller provides several levels of protection to militate against large gauge-head induced pressure bursts that can occur during degas and to protect the vacuum system:

- The emission current is ramped linearly over the degas ramp time. Extended ramp periods (>10mins) ensures gradual gas desorption allowing pumps to handle gas loads.
- Pressures during degas exceeding the **Degas Trip Pressure** parameter value temporarily suspend emission ramping, until the pressure recovers.
- Pressure measurement continues during degas thereby maintaining gauge head trip protection.
- Switching between normal measurement and degas occurs **without** interrupting operation of the gauge.
- A degas sequence cannot be started if the ion gauge is not already operating.
- Degas can be interrupted at any time by selecting a fixed emission current or Auto-emission.

6.7 Ion Gauge Status and Error Messages

Checks are performed on gauge integrity. Status and error conditions include (see also Troubleshooting):

Display	Condition
blank	Ion gauge not connected (interlock not made)
OFF	The ion gauge is off and no error conditions apply
<MinLimit	During ion gauge operation, a collector ion current cannot be measured. [Faulty/disconnected collector lead; collector swamped by electron/ion source]
A/DEr	Fault detected with A/D converter. Ion gauge will be switched off.
HiVer	Fault detected with high voltage (grid) potential [Check rear panel high voltage grid fuse.]
FHiVer	Fault detected with filament potential [Often caused by filament touching chamber wall]
OvrTemp/UndTemp	Internal heatsink over or under temperature condition. Ion gauge switched off.

Fil Er	Ion gauge tripped: filament problem (e.g. open/short circuit filament)
Emiss Er	Ion gauge tripped: emission failed or could not be established.
OvrPres	System pressure too high for ion gauge operation. Ion gauge switched off.
PowerEr	Ion gauge tripped: power output exceeded max power during normal operation setting for > ~30 s. This error condition is not checked during degas as, for very long ion gauge cables, the power needed may exceed maximum voltage available.
DI Er	Digital input assigned to the ion gauge failed, causing the ion gauge to trip out
To OFF	The ion gauge is being powered down.
-> <i>emission</i>	During power up, the initial emission current setpoint value

6.8 PVCduo and Ion Gauge Emission Settings

The high voltage output to the ion gauge grid is protected by a 100mA **fast-blow** fuse to provide instant safety, ion gauge head and controller protection (see section 10). In addition, the controller software places a limit of ~56mA on the current that the ion gauge(s) can draw from the high voltage power supply. In the case of the PVCuni, this has no effect on ion gauge degas under all conditions. However, for the PVCduo, if one or both gauges are set to Degas High (i.e. 50mA emission), the controller will control the emission ramp(s) of the gauge(s) such that the total current drawn does not exceed ~56mA. Aside from this restriction, the ion gauges will continue to operate normally and the degas finish according to its timed schedule.

6.9 Emission Leakage

Ion gauge operation requires good electrical isolation between grid, filament and earth. Gauge feedthroughs can become internally coated causing electrical "leakage" between the pins. Symptoms of leakage include:

- The ion gauge apparently powers up very quickly, or at low filament currents.
- Pressure readings are erratic and very low at low emission currents, or <MinLimit is indicated.

Resistance measurements using a meter may not provide adequate indication of leakage since breakdown/leakage often requires presence of a high voltage. The controller *may* continue to operate a leaky gauge head, but remedial action or replacement of the gauge head is recommended.

6.10 Hints on using ion gauge measurements

The controller has been designed to make use of the ion gauge as simple as possible and provide maximum protection of the ion gauge head and vacuum system. This section provides some hints regarding operation:

6.10.1 Auto-Emission vs Fixed Emission

Wherever possible **use Auto-emission**. The controller will ensure protection and optimal emission current setting to provide good measurement accuracy commensurate with the pressure. The dynamic ion gauge filter algorithm ensures that the controller responds to sudden changes in pressure, for example, due to a pressure burst and will reduce the emission or turn the gauge off to provide protection.

On the other hand, for beam flux measurements require static operating conditions for the ion gauge head; fixed emission may be preferable.

6.10.2 New Filaments – Conditioning and Degassing

New Iridium filaments require "conditioning" as the coating is not initially "activated" until it has been heated for several hours at typical operation temperatures. As a result, the power required to operate a new filament is much higher than after conditioning. In addition, the first time a filament is run, heavy degassing may occur.

6.10.3 Degas

After air exposure, the gauge head requires degassing, e.g. >30minutes emission ramp and >10minutes at DegasHi. This is best performed *after* bake-out of the UHV system, preferably whilst the system is cooling (but >100°C); see section 33 for bake-out auto-degas. Subsequent occasional short degas sequences (5+5 minutes at lower degas power) can keep the gauge operating optimally.

Degassing only affects the currently selected filament. If, a UHV system is to be under vacuum for an extended period, conditioning and degassing *both* filaments after air exposure will minimize subsequent disruption to the vacuum integrity should the second filament be required.

6.10.4 The Ion Gauge Measurement Filtering

Being very small, the collector ion current is prone to disruption from electrical noise. The controller applies to filter to reduce the effects on noise on the pressure reading:

- An input filter applied to the digital measurement of both the collector current and emission current readings. The **Input Filter** parameter is set to a nominal value of 4 and should not need adjusting
- A low pass "smoothing" filter applied to the pressure value. The **LP Filter** parameter can be adjusted between 0.1 and 9.0 s; the default is 1.0 s.

Note that both filters operate "dynamically" and their algorithms interact so that sudden pressure bursts are not ignored and the indicated pressure is accurate at the time of display.

6.11 Ion Current and Beam Flux Measurements

6.11.1 Measurement Method

The controller provides the option to display the ion current value directly. This removes the need to use a separate picoAmmeter, for example, for Beam Flux Measurements (BFM). The controller reads both the emission and ion currents, ensuring that the measurement is compensated for changes in emission (which is not possible if using a separate Ammeter). The measured value can be output from the analogue output and read over comms, for external processing.

To ensure optimal stability of operation of the ion gauge head and controller:

- Set the emission current to a fixed value (usually 10mA) and allow to it stabilize thermally
- Leave the controller on even when the ion gauge is off to maintain thermal stability of the electronics
- Turn the ion gauge on at least 10 minutes before measurements to allow the gauge head to degas

6.11.2 Measuring as Current

For normal pressure measurement (when the ion gauges **IGx Display Units** parameter is set to Pressure) the ion gauge value is displayed in units of mbar, Torr or Pascal, as set by the **Pressure Units** parameter.

The **IGx Display Units** parameter allows the measurement to be presented in Amps in 2 different ways:

- **Electromtr Calib:** This displays the actual ion current being measured (as would a separate picoameter).
- **Ion Current:** The measured current is corrected for emission current and the value normalized to a 10mA equivalent value. When displaying current, the value auto-ranges between units of pA, nA, μ A or mA and data formats of x.xxx, xx.xx, xxx.x.

6.12 Ion Gauge Parameters

The ion gauge has a menu with the following user-definable parameters:

IGx Emission		<p><u>Fixed or Auto-Emission Current:</u></p> <p><u>Off</u> turn the ion gauge off.</p> <p>Fixed emission currents for measurement are <u>0.06mA</u>, <u>0.1mA</u>, <u>0.15mA</u>, <u>0.25mA</u>, <u>0.4mA</u>, <u>0.6mA</u>, <u>1.0mA</u>, <u>1.5mA</u>, <u>2.5mA</u>, <u>4.0mA</u>, <u>6.0mA</u>, <u>10mA</u>. The available fixed emission currents depend on the Minimum and Maximum Emission currents parameter values.</p> <p>Auto-emission current. The control automatically selects the optimum emission current for the pressure range being measured.</p> <p>If the ion gauge is running AND the pressure is below the IG1 Degas Trip parameter value, options to degas the ion gauge at <u>Low Degas</u>, <u>Medium Degas</u> or <u>High Degas</u> powers are also available.</p>
IGx Degas Ramp Time		<p>Degas is a 2 stage process. The emission current is first ramped linearly from its current value to that corresponding to degas power level selected over Degas Ramp Time; during the ramp, the grid voltage is raised to $\sim +400$Vdc. The power is then held for the Degas Hold Time.</p> <p>Each step can be set to have a duration of between 1 and 499 minutes.</p>
IGx Degas Hold Time		
IGx Auto-Degas		<p>The degas level used for automatic degas, for example, optionally at the end of bake-out.</p> <p><u>Low Degas</u>, <u>Medium Degas</u>, or <u>High Degas</u></p>
IGx Degas Trip Level		<p>This has 2 functions:</p> <ul style="list-style-type: none"> - If the pressure is above this level, a degas cannot be started; the 3 Degas Level options will not appear in the IGx Emission parameter menu - If the pressure rises above this level <i>during</i> the degas ramp time, the emission setpoint stops incrementing until the pressure recovers to below this level. However, please note that the degas timer continues to ensure that the degas completes

IGx Min Emission	<i>Note 3</i>	Set the minimum and maximum selectable fixed emission current, and emission current range used during Auto-Emission.
IGx Max Emission		
IGx Min Power IGx Max Power		Set the filament power range used by the PID emission stabilization algorithm. <i>[Defaults of 20 and 60% are suitable for most gauges, but may be varied for small or large gauge heads]</i>
IGx Start Power	<i>Note 1</i>	When powering up the gauge, the controller ramps the power to the filament from 0 to this value. The speed of ramp depends on the Filament Ramp Rate parameter value, which can also be set to "learn" this value automatically. The Start Power cannot be less than the Minimum Power value
IGx Filament Ramp Rate	<i>Note 1</i> <i>Note 3</i>	<u>Standard Ramp</u> : <u>Low Ramp</u> : <u>Fast Ramp</u> : <u>Learn Start Power</u> : The controller performs a slow filament power up, establishes where emission just starts and set this power value to the IGx Start Power parameter. <i>MUST be used with caution on new, unconditioned filaments!</i>
IGx Prop Band IGx Damp	<i>Note 1</i>	Set the gain, integral and differential terms for the PID control of the emission current. <i>[Default values of 25 arbitrary units are suitable for most gauges]</i>
IGx Dig In 1 ... IGx Dig In 4	<i>Note 2</i>	Digital input control over the ion gauge-head <u>None</u> : <u>Interlock</u> : If the digital input fails, the ion gauge turns off <u>Emission On</u> : The ion gauge turns on when the digital input is on, and off when the digital input fails <u>Emission Toggle</u> : A brief (~1second) pulse of the digital input turns the gauge on or off.
IGx Filament Number	<i>Note 3</i>	Selects which filament to use. <u>Auto</u> : Tries filament 1 first and if this fails automatically tries filament 2 <u>1</u> : Uses filament 1 <u>2</u> : Uses filament 2
IGx Sensitivity		The gauge sensitivity value. Range 0.1 to 99.9 mbar ⁻¹
IGx Gas Sensitivity		The sensitivity of the gauge to ambient gas type normalized to Nitrogen having a value of 1. Range 0.01 to 99.99
IGx Filter		Pressure measurement filter. 0.1 to 9.0 s
IGx Input Filter		Reduces low level noise to the collector and emission measurement signals. Range 0 (off) to 9 arbitrary units)
IGx Resolution		Number of decimal places that the ion gauge pressure will be displayed to: <u>1dps</u> or <u>2dps</u> .
IGx Units	<i>Note 4</i>	The ion gauge collector can be displayed a current or as a pressure: <u>Pressure</u> : The ion gauge measurement is displayed as a pressure, normalized to the "global" pressure units selected in the Setup Menu (i.e. mbar, Torr or Pascal). The pressure value is ALWAYS corrected for emission current <u>Electromtr Calib</u> : The ion current (Amps) without correction for emission current <u>Ion Current</u> : The ion current (Amps) after normalizing the emission current to 10mA equivalent
IGx Run Time		<u>Xxx.x hours</u> : The accumulated number of hours of operation of the ion gauge. <u>Reset</u> : Reset the time to zero. For example, after replacing the filament assembly.

Note 1: See section 21

Note 2: Emission On and Emission Toggle are mutually exclusive; Emission On will always dominate

Note 3: Cannot be changed when ion gauge is operating

Note 4: Direct Current and Normalized Current options are suitable for beam flux monitoring applications (BFM)

7 Secondary Gauging

In addition to one (PVCuni) or two (PVCduo) ion gauges, the controller has 2 slots into which modules can be added by the user to support 2 further "secondary" gauge modules. A range of different gauges and types are supported. Secondary gauges can be coupled to the ion gauges, for example, to provide continuous wide-range (UHV to atmosphere) operation (see DGM).

7.1 Secondary Gauge Modules

7.1.1 Module Slots

The controller supports 2 slots into which the user can install "modules" to provide secondary gauging:

- Each module slot comprises a 13 pin in line socket for insertion of the module connector, a support pillar for fixing the module using an M3 bolt and a hole in the rear panel for accessing the module external connector.
- Modules are either 8 pin or 13 pin. They are inserted into the slot connector such that the support pillar aligns with the hole in the module, and the external connector aligns with the rear panel hole - see section 26
- Any combination of modules can be inserted into the slots, with the exception that slot 1 does not accept the "K" module (zone 2 thermocouple 'K' module must be inserted in slot 2)
- After a new module is inserted, the controller will auto-detect the module type and re-configure itself to use the module.

7.1.2 Module Installation


Your controller may have been delivered with specified modules installed. However, modules can be added/removed by the user. The controller will auto-configure itself as required.

Before commencing module installation, turn the controller off and allow 10 minutes for all the high voltage capacitors to discharge FULLY. Place the controller on a bench with the rear panel facing towards you, leaving space on right to lay the lid on the desk as this is attached to the base with an earth wire.


DO NOT CONNECT POWER OR ANY OTHER LEADS TO THE CONTROLLER WHEN OPEN.

DO NOT OPERATE THE CONTROLLER WITH THE LID REMOVED.


AVOID TOUCHING ANY COMPONENT ON THE PCB OR ON THE MODULE - IF AVAILABLE, USE AN EARTHED WRIST STRAP.

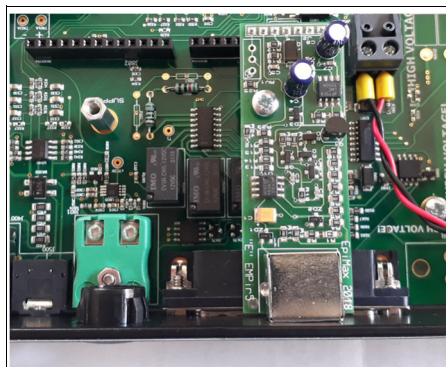

Module 1 installed

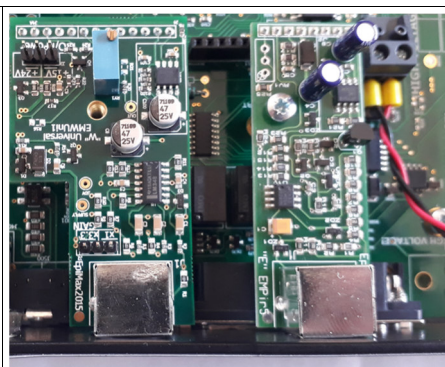

Module 2 positioned

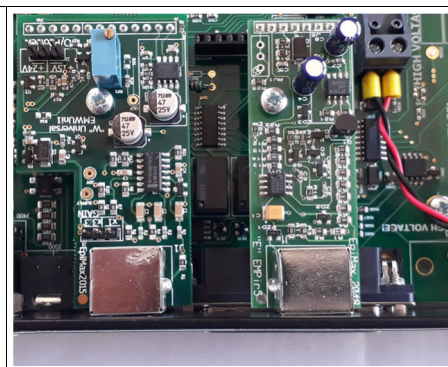

Module 2 installed and secured

INSTALLING A MODULE:

- Remove the 6 off M3 screws securing the lid (3 on each side). Lift the lid carefully, mindful of the earthing wire connecting it to the base; the wire is long enough to lay fold the lid and lay it to the right side of the controller on its top.
- The first picture (above) shows a controller with module in slot 1 already installed, and slot 2 free.
- Note that the rear panel hole for slot 2 is blanked off with a plastic insert. Carefully remove the insert - keep it for future use if a module is to be removed.
- Insert the module into the free socket, second picture above. For 13 pin modules, all 13 pins should engage in the 13 pins of the socket. For 8 pin modules, these should engage with the 8 right hand pins of the socket.
- Ensure that the securing screw hole aligns with the top the support pillar (see second picture above).
- Secure the module in place with the M3 bolt supplied with the module (see third picture above).
- Replace the lid, tucking the earth cable between the transformer and the side of base, and secure with the 6x M3 screws.

REMOVING A MODULE

- Remove the 6 off M3 screws securing the lid (3 on each side). Lift the lid carefully, mindful of the earthing wire connecting it to the base; the wire is long enough to lay fold the lid and lay it to the right side of the controller on its top.
- Unscrew the M3 bolt securing the module to the support pillar (see third picture above).
- Pull the module upwards to disengage its pins from the socket.
- Blank the rear panel hole with a blanking plate.
- Replace the lid, tucking the earth cable between the transformer and the side of base, and secure with the 6x M3 screws.

7.2 Module Types

7.2.1 "E" Module: VSP52x Pirani Gauges

The "E" module supports a VSP52x gauge head; the x in the part number refers to the type of flange (DN16 ISO KF or $\frac{1}{8}$ "NPT) and whether metal sealed. These are half-bridge gauges with built-in temperature compensation. It has a 3 pin mini-DIN connector; note the connector is the same as the "F" module - please ensure you connect the correct gauge type.

VSP52x Pirani gauges are supplied with a 3m connection cable WVSP5003.


Note that Pirani gauge heads have a large tolerance between units, so calibration of the module to match your Pirani head is recommended - see section 12.

7.2.2 "F" Module: VSP84x Pirani Gauges

The "F" module supports a VSP84x gauge head; the x in the part number refers to the type of flange (DN16 ISO KF or $\frac{1}{8}$ "NPT) and whether metal sealed. These are half-bridge gauges with built-in temperature compensation. It has a 3 pin mini-DIN connector; note the connector is the same as the "E" module - please ensure you connect the correct gauge type.

VSP84x Pirani gauges are supplied with a 3m connection cable WVSP8003.


Note that Pirani gauge heads have a large tolerance between units, so calibration of the module to match your Pirani head is recommended - see section 12.

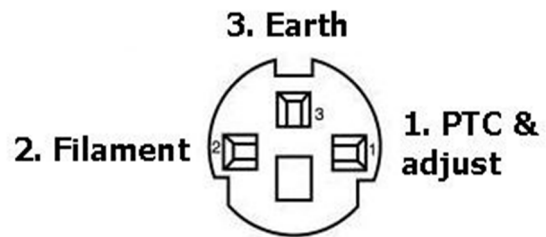

"E" and "F" Module


7.2.3 "W" Universal Module for Linearised gauges

The "W" module has replaced the "U" module, offering additional features and improved specification. It supports a range of active gauge heads, with integrated electronics/cable providing a pressure-linearised output. Pins 1 to 5 offer the same functionality as the "U" module; pin 6 provides a secondary analogue/digital input, see below. The "W" module provides the following:

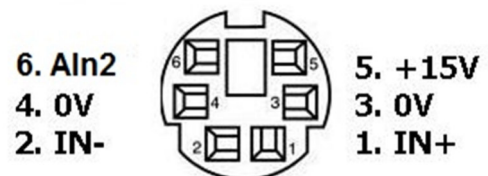

Type "W" Module

- A differential analogue input (pins 2 and 1) from the analogue output of the device. A jumper on the module allows the full scale input range to be selected between 0 to 10V (x1) and 0 to 3.3333V (x3).
- A positive power supply (pin 5) capable of powering the external device. This line is current limited at ~ 120 mA. The output voltage can be selected between +14.5V (nominal) and +24V (nominal) using the "Voltage Out Select" jumper. The higher voltage extends the range of supported devices.
- The output voltage can be switched on and off using the '**W** Power' parameter, allowing the device to be powered only when required. If the external device is always to be powered up when the controller is on, set to **Always On**.
- The '**W** Pull-up' parameter provides a "software" pull-up of the input measurement to maximum value when the module power output is switched off or if the gauge becomes disconnected providing for safe operation of trips associated with the module
- Input voltage and pressure ranges can be set in software to match the output range of the device, or the pressure range of interest (see section "W" Module Parameters)
- The relationship between input voltage and pressure can be set either to logarithmic or linear (see section "W" Module Parameters)
- Pin 6 offers an additional analogue/digital input. The function of this pin awaits implementation in the controller software. Use of screened cable is recommended, with the screen connected to pin 4 of the "W" module.

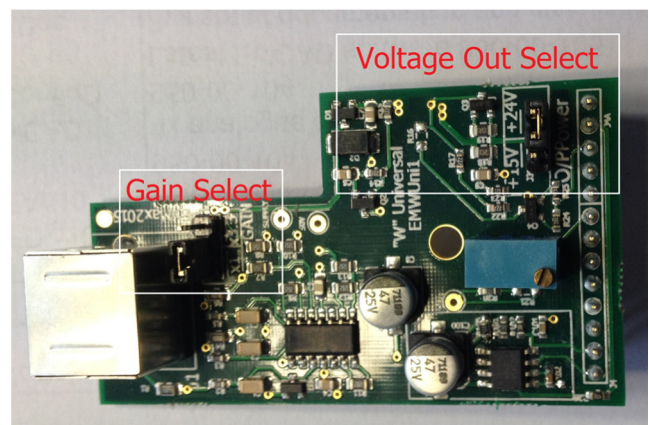

7.3 Module Parameters

7.3.1 "W" Module Parameters

The "W" modules have a menu with the following user-definable parameters:

Power	Turns the power supply to the external gauge (if used) on and off: <u>Off</u> : Power is off. <u>On</u> : Power is on. If the controller is switched off, it will restart with Power Parameter value set to Off. <u>Always On</u> : On controller power up, the power supply is automatically switched on. If this is not set, the power will be off on controller power up
Pull-Up (<i>"W" module only</i>)	If the Power Parameter is set to Off: <u>Off</u> : The module will continue to report the input voltage <u>On</u> : The module will report a "High" reading regardless of the input voltage This eliminates the possibility of a low pressure reading from a gauge if it is intended to be powered by the controller and is inadvertently turned off
Calib Unlock	Unlocks the calibration lock for subsequent parameters. <u>Locked</u> : The parameters are locked, can be inspected but NOT edited <u>Unlocked</u> : The parameters can be edited Note: The calibration lock is reset on returning to the controller Status Mode
Minimum Input Voltage	Voltage corresponding to the Minimum Pressure parameter. Range 0.000V to Maximum Input Voltage parameter value.
Maximum Input Voltage	Voltage corresponding to the Maximum Pressure parameter. Range Minimum Input Voltage parameter value to 9.999V
Minimum Pressure	Pressure value corresponding to the Minimum Input Voltage parameter. Range 1.000e-15 to Maximum Pressure parameter value.
Maximum Pressure	Pressure value corresponding to the Maximum Input Voltage parameter. Range Minimum Pressure parameter value to 1.000e+06
Conversion Function	Relationship between input voltage and Pressures <u>Logarithmic</u> : <i>Pressure</i> proportional to $\log_{10}(\text{input voltage})$ <u>Linear</u> : <i>Pressure</i> proportional to <i>input voltage</i> .

7.3.2 Module Calibration Parameters

Modules interface to external devices, such as gauge heads, outputs from intelligent gauges or controllers. In some cases, particularly Pirani gauge heads, there can be significant differences between performance of individual devices (due to manufacturing tolerance), and performance can change over time.

To address this, all modules can be "calibrated" against known measurement values to match the performance of individual device, using the dual (low and high point) calibration procedures discussed in section 39. Clearly, if a module is replaced and another device attached, calibration values may not apply and recalibration may be necessary.

8 Interlock Hub: Digital I/O and Analogue Outputs

Being user-configurable, the Interlock Hub (which comprises 7 digital output trips, 4 digital inputs and 2 analogue outputs) relate the pressure/temperature measurements to various aspects of system operation (pumps, valves...). The hub can largely replace interlock wiring, and provides versatile implementation of interlocking and bake-out heater control.



Note: The controller Interlock Hub is NOT a substitute for hard-wire interlocking where safety, high level security, or potentially hazardous situations can arise. No liability is accepted for problems caused by inappropriate use of the controller.


8.1 Trips (Digital Outputs)

There are 7 trips: trips 1 to 4 are relay-based and trips 5 to 7 open-collector NPN Darlington outputs.

8.1.1 Relay-based Trips 1 to 4

SPCO (single-pole, change-over) relays, rated at 1A@24Vdc, and 0.5A@40Vac. The minimum switching current is 1mA@5Vdc. When using the relay outputs with inductive (e.g. relays or valve solenoids) or capacitive loads, suppression of back emf or current surges **MUST** be employed:

- (a) Drive of a resistive load: e.g. TTL input. Note that the value of R must be sufficiently low to ensure that at least 1mA flows through the relay contacts. Using the normally open contact inverts the signal.
- (b) Switches a contactor with dc coil, for example, to a heater. To comply with the 1A contact current limit, the resistance of the external relay coil must be $>30\Omega$. The reverse biased diode **MUST BE PRESENT** to suppress the back emf generated by the inductive load presented by the relay coil; this diode requires a reverse voltage rating $>> +24V$ supply, and a current rating at least twice that consumed by the relay coil. The 1N4001 is suitable for supplies up to about 40V.
- (c) Switches a contactor with ac coil. An RC snubber network **MUST BE** used for back-emf suppression. Typical R and C values are 100Ω and $0.1\mu F$; composite snubbers components are available.

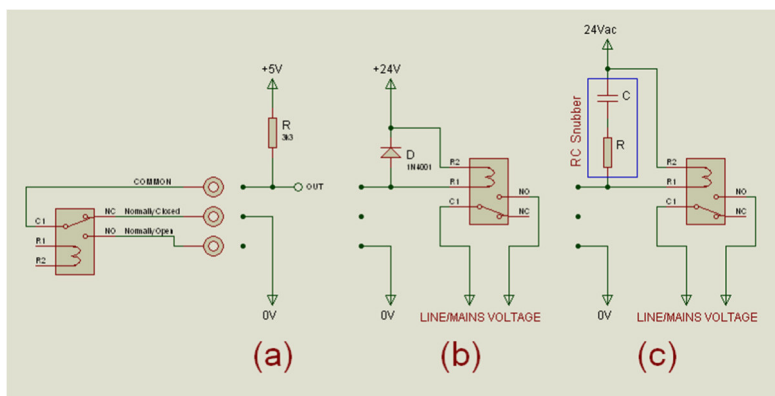

8.1.2 Open Collector-based Trips 5 to 7


DO NOT USE APPLY $> +14V$ TO TRIPS 5 to 7.

Open-collector Darlington transistor output, each capable of sinking 200mA at 12Vdc. **Only dc devices can be driven with these outputs. The outputs are 0V (earth) referenced.**

The output configuration is shown on the left of the diagram. A built-in protection diode connected to the internal +12V supply limits the voltage to the driven devices (the potential at the outputs) to just over 12Vdc.

(a) Shows a scheme for driving a 5V TTL, or similar, load. As the output from a Darlington transistor at $\sim 1V$ exceeds the low logic threshold of some logic families, a transistor buffer is used. This also inverts the signal so that the output is high when the trip is on.

(b) Shows the output driving a relay, e.g. for mains switching. Note that despite the presence of an internal diode, an external diode is required across the relay coil for emf suppression **to the relay supply rail**.

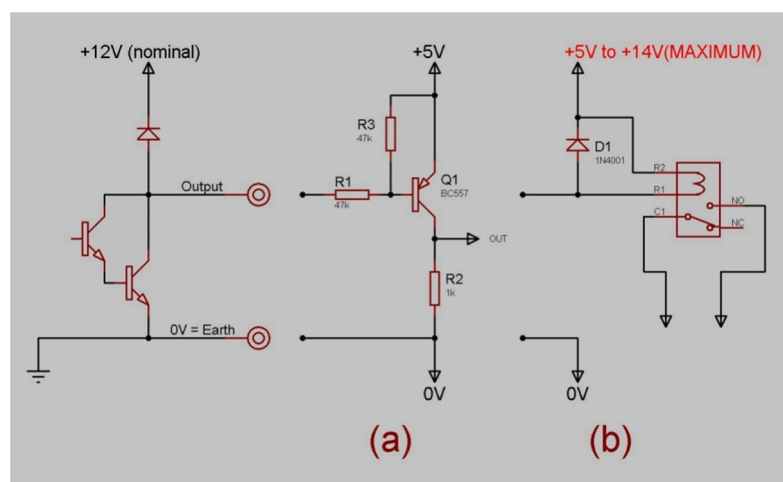

8.1.3 Trip Parameters

Each Trip has a menu with the following user-definable parameters:

State	Trip : the trip state is determined by its allocation Inhibit : the trip is off Override : the trip is on
--------------	---


Power-up State	<p><u>Last Setting</u>: On power up, the trip resumes the state it had powered down.</p> <p><u>Reset On Power Up</u>: On power up, an inhibit or override state current when powered down is removed</p> <p><u>Inhibit</u>: The trip will power up in the inhibit state</p> <p><u>Override</u>: The trip will power up in the override state</p>
Allocation	<p><u>None</u>: The trip is not used</p> <p><u>IG1 Pressure</u>: The trip is triggered by ion gauge 1 at its trip point</p> <p><u>Module 1</u>: The trip is triggered by the device connected to module 1 at its trip point</p> <p><u>BakeOut Zone1</u>: The trip is triggered by bake-out temperature control for zone 1</p> <p><u>Module 2</u>: The trip is triggered by the device connected to module 2 at its trip point</p> <p><u>IG1 DGM Pressure</u>: The trip is triggered by the ion gauge 1 operating in dual gauge mode at its trip point</p> <p><u>IG1 On</u>: The trip is when when ion gauge 1 is operating</p> <p><u>IG1 Degas</u>: The trip is when when ion gauge 1 is degassing</p> <p><u>BakeOut Zone2</u>: The trip is triggered by bake-out temperature control for zone 2</p> <p><u>Timer 1</u>: The trip is on during the on period of timer 1</p> <p><u>Timer 2</u>: The trip is on during the on period of timer 2</p> <p><u>Live Heartbeat</u>: The output changes state every second as indicator that controller operating (<i>open collector trips 5, 6 and 7 only</i>)</p> <p><u>IG2 Pressure</u>: The trip is triggered by ion gauge 2 at its trip point (<i>duo only</i>)</p> <p><u>IG2 DGM Pressure</u>: The trip is triggered by the ion gauge 2 operating in dual gauge mode at its trip point (<i>duo only</i>)</p> <p><u>IG1 On</u>: The trip is when when ion gauge 1 is operating (<i>duo only</i>)</p> <p><u>IG2 Degas</u>: The trip is when when ion gauge 2 is degassing (<i>duo only</i>)</p>
Direction	<p>\leq The trip is on when the allocation is below the "Trip at" parameter value</p> <p>\geq The trip is on when the allocation is above the "Trip at" parameter value</p>
Trip at	For gauge type allocations, the pressure at which the trip operates, moderated by the hysteresis parameter
Trip Hysteresis	To avoid trip on/off "chatter" when the pressure value is near the trip value, the off trip value is higher than the on trip value by a factor defined in this parameter. For example, setting the value to 1.5x sets the off trip value to 1.5x the trip at value. Note that this parameter is common to all the trips.

8.2 Digital Inputs

8.2.1 Digital Input Hardware

The diagram shows the equivalent circuit for the 4 digital inputs, as well as the drive circuitry that can be optionally used to drive the inputs:

- All digital inputs are opto-isolated from the controller electronics.
- Diodes protect against reverse connection.
- Digital inputs 1 and 2 are isolated, whereas digital inputs 3 and 4 share a negative terminal
- The input voltage range is ~3 to 30Vdc (limited by power rating of the input resistor). If higher voltages are to be used, add a series resistor to limit the input current to 10mA.
- The inputs can be driven directly from most 5 – 15V logic families (TTL, CMOS...), or from an external power supply switched through a relay or contactor.
- Alternatively, pins 11 and 7/23 provide an internal current limited supply that can be used to drive the digital inputs, for example, switched through a relay. Please note that care is needed to ensure that this internal supply is not inadvertently connected to an external supply.

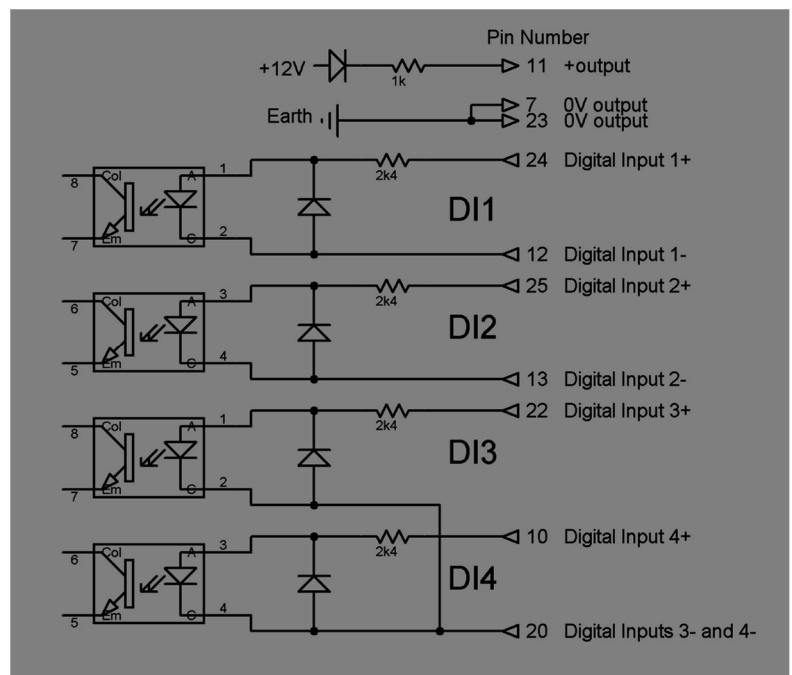

8.2.2 Digital Input Parameters

Each Digital Input has a menu with the following user-definable parameters:

State	<u>Trip</u> : the input voltage determines if the digital input is off or on. <u>Inhibit</u> : the digital input is off, regardless of the input voltage <u>Override</u> : the digital input is on, regardless of the input voltage
Power Up State	<u>Last Setting</u> : On power up, the digital input will have inhibit or override state it had when powered down. <u>Reset On Power Up</u> : On power up, the digital input is reset to trip state <u>Inhibit</u> : The digital input will power up in the inhibit state <u>Override</u> : The digital input will power up in the override state
Invert	<u>Normal</u> : A voltage applied to the digital input turns it on; the default state is off <u>Invert</u> : A voltage applied to the digital input turns it off; the default state is on

8.2.3 Digital Input Applications

Digital inputs can be used to interlock the following:

- **Ion gauge(s)** interlocking, switching on and off and degas on and off
- **Bake-out**. Individual digital inputs can be used independently to inhibit the heater output, suspend the bake-out (i.e. inhibit the heater output and pause the bake-out timer) or terminate the bake-out.
- **Timers**. Individual digital inputs can be used independently to inhibit the ON time output

Please refer to the parameters for each of these for further information.

8.3 Interlock Hub Status Page

The Interlock Hub Status Page provides a summary of the trip and digital input states:

```

:Tr: On  Off  Inh  On  Ovr  Off  Off
:DI: On  On  Off  Inh
  
```

If the **CANCEL** button is pressed and held, the display scrolls through the 7 trips and 4 digital inputs providing information about trip allocation and digital input usage:

```

:Tr: Trip4 Off - IG1 Pressure
:DI: DI2 On  - IG1:Bake;
  
```

The example above indicates that:

- Trip 4 is currently off and is allocated to IG1 pressure.
- Digital Input 2 is used to interlock both IG1 and Bake-out.

8.4 Analogue Outputs

The two analogue outputs share a stereo (3 pin) jack-plug output. If a mono (2 pin) jack-plug is used, ensure that analogue output 2 Allocation is set to "OFF" to avoid accidentally electrically "shorting" the output.

8.4.1 Overview

The controller has 2 independent analogue outputs (AOs). Each AO is designed to provide up to ~10.2V and is factory calibrated (using the Calibrate menu - see section 40) to provide a range of 0 to 10.00V; this can subsequently be adjusted by the user.

The maximum current available from the output is ~20mA. However, to avoid excessive power dissipation of the output

amplifiers, please heed of the warning at the start of this section.

The AOs are user configurable by setting the minimum and maximum voltage to scale with the minimum and maximum pressure to be monitored. The relationship between pressure and voltage can be set to either Logarithmic or Linear. In addition, the AOs can be inhibited by the digital inputs (see section 32).

8.4.2 Analogue Output and Ion gauge Allocation

An AO allocated to an ion gauge follows the measured pressure when the ion gauge is on. However, when the ion gauge is not operating, the AO outputs either the **Maximum** or **Minimum Output Voltage** parameter value, depending on the setting of the **Fail to** parameter setting. For most applications where failure of vacuum is the fault condition, this should be set to Fail To Maximum Output Voltage.

8.4.3 Digital Input Interlocking of Analogue Outputs

The **DIx Interlock** parameters allow one or more of the digital inputs to inhibit the AO. When inhibited, the AO outputs either the **Maximum** or **Minimum Output Voltage** parameter value, depending on the setting of the **Fail to** parameter setting.

8.4.4 Analogue Output Parameters

Each Analogue Output has a menu with the following user-defined parameters:

Allocation	Set to Min Out : Output set to minimum output parameter value Set to Max Out : Output set to maximum output parameter value IG1 Pressure* : Output voltage reflects the ion gauge 1 value DualIG1 Pressure* : Output voltage reflects the ion gauge 1 dual gauge value Module 1 : Output voltage reflects the device attached to module 1 value (<i>if module 1 fitted</i>) Module 2 : Output voltage reflects the device attached to module 2 value (<i>if module 2 fitted</i>) Thermocouple : Output depends on the measured thermocouple value. Depends on the minimum output, maximum output, minimum and maximum pressure (interpreted as temperature) and log/lin parameter values Comms External : The output value is set directly to match the value set over comms Off : Analogue output not used. Output value set to 0.0V IG2 Pressure : Output voltage reflects the ion gauge 2 value (<i>duo only</i>) DualIG2 Pressure : Output voltage reflects the ion gauge 2 dual gauge value (<i>duo only</i>)
Pressure Minimum	The pressure value that the minimum voltage parameter corresponds to. Range 1.000e-16 to Maximum Pressure
Pressure Maximum	The pressure value that the maximum voltage parameter corresponds to. Range Minimum Pressure to 1.000e+6
Minimum Output Voltage	The output voltage (in <i>milliVolts</i>) that the minimum pressure parameter corresponds to. Range 0 to Maximum Output Voltage
Maximum Output Voltage	The output voltage (in <i>milliVolts</i>) that the maximum pressure parameter corresponds to. Range Minimum Output Voltage to 9999mV
Function	Defines the relationship between the pressure and voltage output. Either Logarithmic or Linear
Fail to:	Max Output : The failed state of the analogue output is the Maximum Output Voltage parameter value. Min Output : The failed state of the analogue output is the Minimum Output Voltage parameter value. For discussion of the "failed" state, please refer to sections 32 and 32.
DI1 Interlock	OFF : No effect. The AO follows the allocated device Inhibit : The AO outputs the Maximum Output Voltage parameter value
DI2 Interlock	
DI3 Interlock	
DI4 Interlock	

9 Bake-out Control


The controller has a multi-step ramp/soak bake out sequencer which integrates pressure and external interlocking, and provides auto-degassing of ion gauge.

9.1 Overview

The schematic represents the single- and dual-zone bake-out operation. The pink blocks represent the components for the first zone bake-out available as standard on the controller. By addition of a 'K' module in slot 2 (see section xxx), a second bake-out zone (represented by the green blocks) becomes available.

Key features:


- Up to 6 ramp/soak periods, each step up to 99:59 hours:mins.
- Each zone has its own definable 6 step temperature profile.
- Any combination of the 7 trips can be assigned to either zone to switch the heaters
- Digital inputs, ion gauge(s) can be individually set to inhibit (trips off), suspend (trips off and suspend bake-out timer) or terminate the bake-out
- Zones can be run individually or simultaneously.
- Optional auto-degassing of ion gauge(s) at the end of bake-out
- As well as setpoint, measured value, remaining time and step number for each zone, the peak temperatures reached during the bake-out are recorded and accessible from the display and over communications.

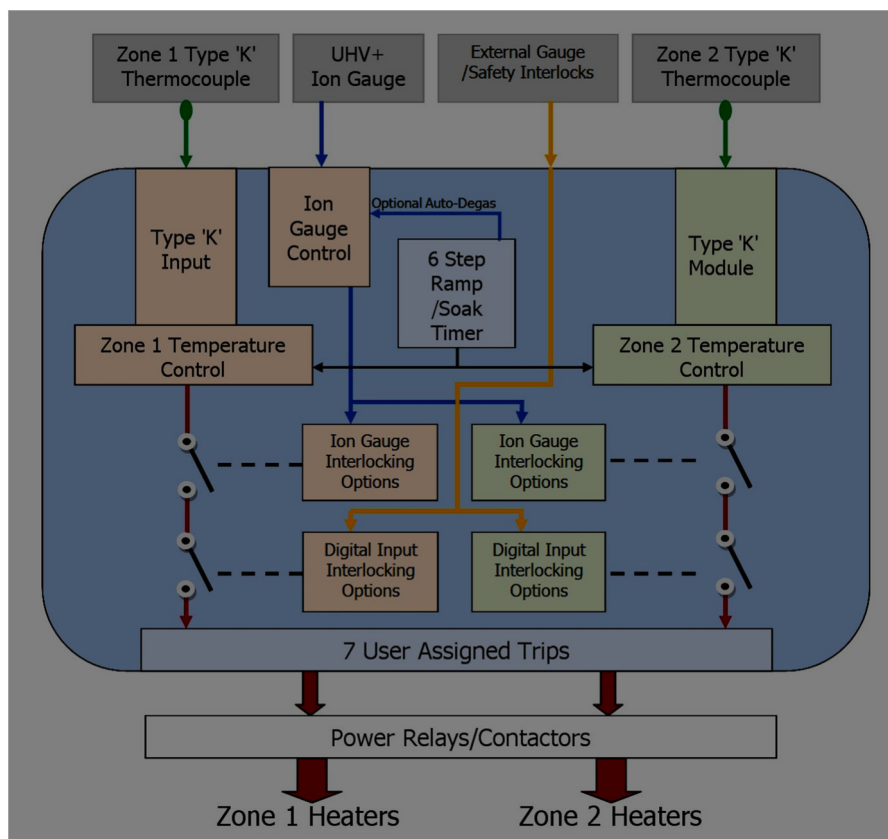

9.2 Temperature Profile

The graph, right, is an example of a 5 step bake-out temperature profile (step 6 is ignored by setting its time to 00:00). The graph shows that during the first step, the temperature setpoint rises linearly from the current measured value to the step 1 value (120°C) in 1 hour. As the step 2 temperature is the same as step 1, the setpoint is then held for 3 hours. In step 3, the temperature ramps to 220°C over a period of 2 hours, is held there for 14 hours in step 4 and finally ramped back down to room temperature in step 5.

The use of temperature ramps helps avoid pressure bursts during heating and temperature overshoot.

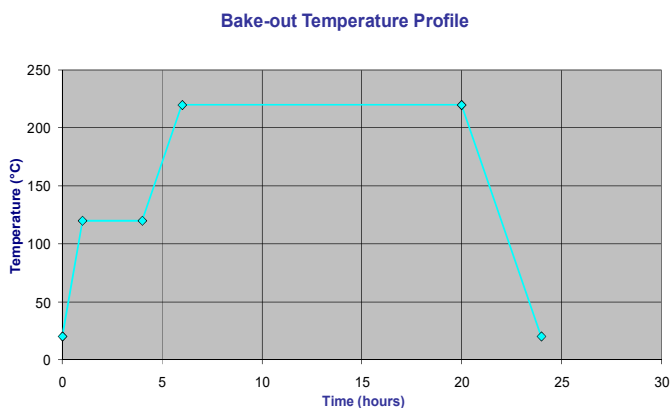

9.3 Bake-out Interlocking

Bake-out operation can be influenced by the digital inputs and ion gauges, or by user intervention – see the bake-out parameters. There are 3 levels of interlocking:

- **Inhibit.** Allocated trip operation is set to off. However, the bake-out timer continues.
- **Suspend.** As well as setting the allocated trips to off, the bake-out timer clock is suspended until the interlocks are cleared
- **Suspend.** As well as inhibiting the allocated trips, the bake-out time is suspended whilst the interlock is failed
- **Terminate.** The bake-out is terminated. If ion gauge auto-degas is set, it is NOT executed

9.4 Display of Bake-out Operation

Bake-out has a dedicated Status screen, for example:

```

:Bake-Out Step 3 Time 012:02:30hms
:Z1: 194.0/ 193.7°C ON
  
```

```

:Bake-Out Step 3 Time 012:02:30hms
:Z1: 194.0/ 170.3°C (sus) DI
  
```

- The top line indicates the currently executing step number and the **remaining** time for the bake-out
- The bottom line indicates the currently displayed zone; if 2 zones are executing, the display toggles between the 2 zones. This is followed by the Setpoint/Measured value and the trip states. The first image shows that allocated trips are ON, whereas the second image shows that bake-out is suspended due to a digital input failure.

Pressing the **CANCEL** button displays the peak temperatures for both zones during the present or previous bake-out:

```

:Bake-Out OFF
:Z1 PeakT 202.0°C Z2 PeakT 183.0°C
  
```

In addition, bake-out is indicated in other Status screens. If a zone 1 bake-out is in progress, the thermocouple name is inverted, and if zone 2 bake-out is in progress, the module 2 name is displayed.

9.5 Bake-out Parameters

The bake-out menu provides the following user-definable parameters:

BO Start/Stop		---: No action <u>Start Zone 1:</u> Start bake-out zone 1 profile only <u>Start Zone 2:</u> Start bake-out zone 2 profile only. {Only available if module 2 is fitted with "K" module} <u>Start Zones 1&2:</u> Start bake-out, both zones. {Only available if module 2 is fitted with "K" module} <u>STOP:</u> Stops the bake-out Note: Zone 1 cannot be started if thermocouple is its disconnected. Zone 2 cannot be started if no 'K' module in slot 2, or its thermocouple is disconnected.
BO User Interlock		Allows the user to temporarily inhibit or suspend the bake-out <u>OFF:</u> No user action <u>Inhibit:</u> Trips turned off <u>Suspend:</u> Trips turned off and bake-out timer is suspended
BO Step1 Time BO Step6 Time		Step duration. Value: 00:00 to 99:59 hm.
BO Z1 Step1 Temp BO Z1 Step6 Temp		Zone 1 temperature attained at the end of the step. Value: 1 to 500°C. If different from previous step, the temperature is linearly ramped from the previous value.

BO Hysteresis		To avoid on/off switching (contact chatter), the trip turn-on temperature = zone setpoint and the trips turn-on temperature = (zone setpoint + hysteresis value). Value: 0.1 to 9.0°C.
BO Z2 Step1 Temp BO Z2 Step6 Temp	<i>Note 2</i>	Zone 2 temperature attained at the end of the step. Value: 1 to 500°C. If different from previous step, the temperature is linearly ramped from the previous value.
BO DI1 Interlock BO DI4 Interlock		<u>OFF</u> : No operation <u>Inhibit</u> : Trips turned off <u>Suspend</u> : Trips turned off and bake-out timer stopped <u>Terminate</u> : Terminates the bake-out, turning all allocated trips to off, and resetting zone setpoints Note: Different digital inputs can be set to perform different functions
BO IG1 Interlock		<u>OFF</u> : No operation <u>Inhibit</u> : Trips turned off <u>Suspend</u> : Trips turned off and bake-out timer stopped <u>Terminate</u> : Terminates the bake-out, turning all allocated trips to off, and resetting zone setpoints
BO IG1 Pressure Trip		Ion gauge 1 interlock pressure value. If exceeded, the ion gauge interlock operates
BO IG1 AutoDegas		Auto-start degas of ion gauge 1 at its Auto-degas parameter setting at the end of bake-out
BO IG2 Interlock	<i>Note 1</i>	<u>OFF</u> : No operation <u>Inhibit</u> : Trips turned off <u>Suspend</u> : Trips turned off and bake-out timer stopped <u>Terminate</u> : Terminates the bake-out, turning all allocated trips to off, and resetting zone setpoints
BO IG2 Pressure Trip	<i>Note 1</i>	Ion gauge 1 interlock pressure value. If exceeded, the ion gauge interlock operates
BO IG2 AutoDegas	<i>Note 1</i>	Auto-start degas of ion gauge 1 at its Auto-degas parameter setting at the end of bake-out

Note 1: Only available for PVCduo

Note 2: Only available if K module installed in Slot 2

10 Dual (wide-range) Gauge Mode

Dual Gauge Mode combines the ion gauge with a module-based gauge so they operate as a single pressure measurement device.

10.1 Overview

Dual Gauge (DGM) is a special controller mode in which ion gauge operation is combined with a secondary gauge (**SG**) so they operate as though they were a single gauge head from the point of view of pressure display (and optionally) trip setting. The ion gauge automatically starts and stops depending on user-defined parameters. This allows continuous monitoring of the pressure over a wider range than available to just the ion gauge, for example, all the way from atmosphere to UHV.

The PVCuni ion gauge can be combined with a module in either slot. Similarly, either PVCduo ion gauge can be combined with either module, but both ion gauges cannot be combined with the same module. Once a module is assigned to an ion gauge (**DGM Assign**), DGM operation can be enabled and disabled as required (**DGM Operation**).

The way DGM operates is as follows:

- Assuming the ion gauge is off, the pressure read by the SG will be reported for the ion gauge.
- If the SG pressure falls below the **DGM Gauge On** parameter value, the controller waits for a period defined by the **DGM Delay** parameter and then attempts to start the ion gauge at the **DGM Emission** parameter value (usually set to Auto-emission).

- If successful, the ion gauge reports its own reading.
- If not successful (e.g. because the pressure is not low enough for ion gauge operation), the controller will repeat the attempt the number of times set by the **DGM Attempts** parameter.
- If, during ion gauge operation, the ion gauge pressure rises above the **DGM Gauge Off** parameter value, the ion gauge turns off and the SG pressure is reported for the ion gauge.
- In the addition, the **DGM SG Protect** parameter optionally defines whether the SG pressure value is monitored for exceeding the off pressure, as well as the ion gauge pressure.

The **DGM Options** parameter defines how and when DGM will operate:

- **Enabled at Power Up:** If a DGM SG is assigned and enabled for operation, this option will start DGM processing as soon as the controller is switched on.
- **Disabled at Power Up:** If a DGM SG is assigned and enabled for operation, the controller will set the **DGM Operation** parameter to disabled on power up.
- **Once: Pump Down:** Once the ion gauge has been started successfully through DGM processing, the **DGM Operation** parameter is disabled to inhibit any further DGM action

When DGM is operating, the third character in the ion gauge's name is changed to '*'. For example, for "IG1", the name appears in all screens as "IG*".

10.2 DGM and Menu Parameters

The DGM menu(s) provide the following user-definable parameters. Note that the parameter name is preceded by the name of ion gauge (e.g. "LL DGM Operation"):

DGM Operation	Disabled: DGM not operating Enabled: DGM operating if a DGM Assign parameter is set.
DGM Assign	OFF: Not assigned. DGM not operational <i>ppp + ss1</i> : Gauge in slot 1 is assigned to the ion gauge (only appears if a suitable module is present) <i>ppp + ss2</i> : Gauge in slot 2 is assigned to the ion gauge (only appears if a suitable module is present)
DGM Options	Disabled at Power Up: Enabled at Power Up: Once: Pump Down: Please refer to section 35 for details
DGM SG Protect	Off: During ion gauge operation, only the ion gauge pressure is tested against the DGM Gauge Off parameter value for turning the ion gauge off. On: During ion gauge operation, both the ion gauge and SG pressures are tested against the DGM Gauge Off parameter value for turning the ion gauge off.
DGM Gauge On	The SG pressure value at which the ion gauge can be turned on. Note: the controller does not allow this value to be greater than the DGM Gauge Off value.
DGM Gauge Off	The ion gauge (and optionally SG) pressure value at which the ion gauge is turned off. Note: the controller does not allow this value to be less than the DGM Gauge On value
DGM Emission	The emission at which the ion gauge will operate during DGM processing (usually Auto-emission)
DGM Delay	Once the DGM Gauge On pressure has been reached, the controller will wait for the specified period before attempting to start the ion gauge. If, during this period, the pressure goes above the gauge on value, the process for testing restarts. Range: 0.0 to 499.0 seconds.
DGM Attempts	The number of attempts DGM processing will make to start the ion gauge. Once the ion gauge is started, the attempt count is reset to zero for the next cycle. If the ion gauge cannot be started after the specified number of attempts, DGM operation is disabled

10.3 Safe DGM Operation

- **DGM MUST be used with a combination of ion gauge and secondary gauge mounted *within the same vacuum envelope*.** The presence of an isolating valve between the two would clearly preclude sampling the vacuum. The only exception is if used with the "Once Pump Down" option where isolation between, say a vacuum chamber and its evacuation/backing line is required at the end of the pump-down cycle and DGM processing then ceases.
- If using a secondary gauge is a powered device, ensure that the gauge is suitably powered **at all times**. For example, if using a gauge connected to and powered by a "W" module, ensure that the "W" module **'W' Power** parameter is set to "Always On". It is advisable to also set the **'W' Pull-up** parameter to ON so that high pressure is indicated if the gauge is disconnected.

- To preclude "hunting", ensure sufficient hysteresis between the **DGM Gauge On** and **DGM Gauge Off** parameter values. The controller will in any case not allow the pressure off value to exceed the pressure on value.

10.4 Auto-cancellation of DGM Operation

For safety reasons, DGM operation is automatically disabled under the following conditions:

- If no ion gauge is connected
- If the ion gauge is turned off by the user either from the front panel or over comms
- If the ion gauge fails to start after the specified number of attempts

11 Timers 1 and 2


A new feature to the PVC range is inclusion of 2 timers, which can be used to drive external events as one-shot or cyclical operations: firing TSP pumps, auto-opening valves during work periods, triggering pump/degas cycles, to automatically closing a valve after a period of time has elapsed...

11.1 Overview

The controller has two independent timers that can be used to trigger external events, via allocated trips, either just once or on a repeating cyclical basis. The user can intervene at will to modify timer operation, and optional digital input and ion gauge interlocks can automatically provide protection.

Timers can be "one-shot" (they run once and terminate) or cyclical (they repeat until terminated by the user or an interlock).

When running, a timer can be restarted at the start of the off, or the start of the on time, or at any other point in its cycle time.

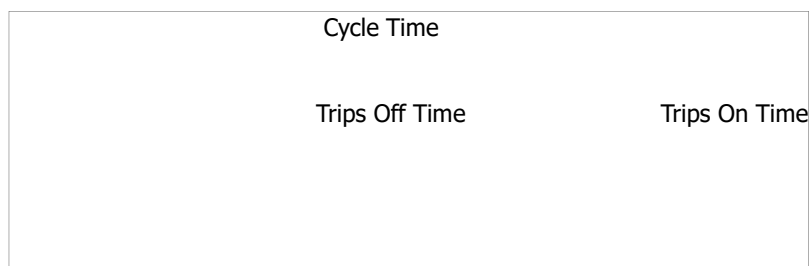

11.2 Timer Interlocking

Timer operation can be influenced by the digital inputs and ion gauges, or by user intervention – see the timer parameters, section 11.4. There are 3 levels of interlocking:

- **Inhibit.** Allocated trip operation is set to off. However, the timer clock continues.
- **Suspend.** As well as setting the allocated trips to off, the timer clock is suspended until the interlocks are cleared
- **Terminate.** The timer operation is terminated

11.3 Timer Status Display

Bake-out has a dedicated Status screen, for example:



This shows the status of both timers. In the example above:

- Timer 1 is not operating
- Timer 2 is at 15:10 in its cycle. The ON message indicates that it is within the trips on time and the allocated trips are ON.



- This image shows that Timer 2 is at 6:30 in its cycle. The (on) message indicates that it is within the trips on time; however, the trips are off due to a digital input interlock failure indicated by **DI**.

Pressing the **CANCEL** button provides the main settings for the timers, namely the type of timer and the cycle time:



11.4 Timer Parameters

Each Timer has a menu with the following user-defined parameters

Tmr\times Type		One-Shot : The timer runs once and automatically terminates Cyclical : Once reaching the end time, the timer repeats indefinitely The type can be changed during timer operation
Tmr\times Operation		--- : No action Set@ OFFTime : (Re-)Start the timer at the start of the off time Set@ ONTime : (Re-)Start the timer at the end time parameter value (i.e. the start of the on time) Set@ RESTARTTime : (Re-)Start the timer at the point in the cycle defined by the timer Restart parameter STOP Timer : Cancels timer operation
Tmr\times User Inhibit		Allows the user to temporarily inhibit the timer trip outputs OFF : No action Inhibit : Trips turned off Suspend : Trips turned off and the timer is suspended
Tmr\times Cycle Time		The total (off + on) time. 000:00:01 to 999:59:59 hms
Tmr\times Off Time		The time the trips allocated to the timer remain off, i.e. the start of the on time 000:00:01 to the Cycle Timer parameter value
Tmr\times Restart Time		The restart time used for the Set@ RESTARTTime setting the restart time to an arbitrary value using the Tmr Operation Set@ RESATRTime parameter value
Tmr\times DI1 Interlock Tmr\times DI4 Interlock		Sets the digital input action on the timer trip outputs OFF : No action Inhibit : Trips turned off by the DI Suspend : Trips turned off and the timer is suspended Terminate : Terminates the timer turning all allocated trips to off Note: Different digital inputs can be set to perform different functions
Tmr\times IG1 Interlock		Sets whether ion gauge 1 inhibits the timer trip outputs if above the pressure set in the Tmr IG1 Pressure parameter OFF : No action Inhibit : Trips turned off by the ion gauge Suspend : Trips turned off and the timer is suspended Terminate : Terminates the timer turning all allocated trips to off
Tmr\times IG1 Pressure		The pressure value at which the ion gauge 1 inhibits the timer trip outputs
Tmr\times IG2 Interlock	<i>Note 1</i>	Sets whether ion gauge 2 inhibits the timer trip outputs if above the pressure set in the Tmr IG2 Pressure parameter OFF : No action Inhibit : Trips turned off by the ion gauge Suspend : Trips turned off and the timer is suspended Terminate : Terminates the timer turning all allocated trips to off
Tmr\times IG2 Pressure	<i>Note 1</i>	The pressure value at which the ion gauge 2 inhibits the timer trip outputs

Note 1: PVCduo only

12 Calibration

The controller is calibrated against "standards" during manufacture. However, gauge heads vary significantly due to their structure. The methods available to the controller to match specific gauge heads is discussed.

12.1 Calibration

The controllers are calibrated during final testing before dispatching to remove the effects of component and design tolerance. However, there are 2 circumstances where re-calibration may be necessary:

- All electronics can "drift" with time, or when used at extremes of temperature. Although this is usually a small effect and should not be a requirement within the lifetime of the controller.
- The electronics may need calibration to "match" the behaviour of a specific device. For example, due to manufacturing tolerance, Pirani gauges of the same type can differ by up to 5% between units.

The PVC controllers provide the facility for the user to execute calibration.

There are 2 types of calibration:

- Single High point or "gain" calibration used for calibrating the two analogue outputs
- Low and High dual point calibration used to calibrate thermocouples, and gauge modules such as the 'E', 'F' and 'W'.

12.2 High Point (Gain) Calibration of Analogue Outputs

This entails measuring the analogue output voltages on a calibrated voltmeter whilst adjusting the calibration parameter:

- From the relevant Analogue Output Menu, set the **Maximum Output** parameter to a high value (we recommend using the maximum 9999mV)
- Also set the **Allocation Parameter** to "SetToMaxOut"
- Enter the Calibration Menu and unlock it (see section 12.4)
- Scroll to the relevant parameter (either **AO1** or **AO2 Calibrate High**) and adjust the value so you meter reads as close to 9.999V as possible. Note that the designed full range for the analogue outputs is 0 to ~10.2V, so typical calibration values are in the range -200 to -240 (nominal mV).
- Restore the **Maximum Output** and **Allocation Parameters** for the analogue output

12.3 Low and High Dual Point Calibration

The Low/High calibration is a two-step process where separate low and high value adjustments are made. They require some independent measurement or knowledge of the devices being calibrated with. This applies to thermocouple inputs and all secondary gauges attached to 'E', 'F' and 'W' modules.

All Low and High Calibration have a "neutral" (i.e. no correction) value of **5000**; calibration involved adjusting the values over the range 1 to 12000 to match the "correct" value.

With Low/High calibration, as well as the value of the calibration parameter, the actual current measurement is also displayed, for example, for a Pirani calibration:



The image shows a yellow LCD display with black text. The top line reads 'LL1 HIGH Calib'. The second line shows '1.00E+03' on the left and '5000' on the right, followed by a question mark.

As the adjustment procedure is the same for all devices is the same, we will take the example of calibrating a 521 Pirani gauge head attached to an 'E' module. Note that calibration of Pirani's is particularly sensitive due to their poor resolution in output at the extremes of the measurement range.

Calibration at Atmosphere

For Pirani gauges, it is suggested that calibration at atmosphere be performed first. Vent the Pirani gauge chamber and allow a few minutes to settle.

- Enter the Calibration Menu, and unlock calibration (see section 11.4)
- Select the relevant **HIGH Calib** Parameter:



The image shows a yellow LCD display with black text. The top line reads 'LL1 HIGH Calib'. The second line shows '1.00E+03' on the left and '5100' on the right, followed by a question mark.

Note that in this case, the indicated pressure appears to be below 1.00E3 mbar (atmosphere).

- Adjust the Calibration Parameter value so that the indicated pressure just moves just above and below atmosphere.

Calibration at Vacuum

- Evacuate the Pirani chamber, allowing it to settle at a known pressure, or below the measurement range of the Pirani.
- Select the **LOW Calib** Parameter for the device
- If calibration is against a known reference, for example, another gauge or the minimum pressure for a rotary backing pump, adjust the calibration parameter to indicate that value
- If calibration is at a pressure below the minimum for the Pirani (1e-4mBar), adjust the calibration parameter to indicate as close to 1e-4mBar as possible.

12.4 Calibration Menu Parameters

To avoid “accidental” changes to calibration parameter values, on entering the calibration menu all parameters (except the first) are locked, as indicated by the key symbol adjacent to the parameter value. This indicates that the parameter value cannot be changed:



To access editing of the parameter values in the calibration menu, the **Calib Unlock** parameter (the first parameter) needs to be changed from “locked” to “unlocked” as indicated by the change from a key to an editing symbol:



Calib Unlock		Unlocks the calibration lock for subsequent parameters. <u>Locked</u> : The parameters are locked, can be inspected but NOT edited <u>Unlocked</u> : The parameters can be edited Note: The calibration lock is reset on returning to the controller Status Mode
T/C HIGH		Dual low and high point calibration parameters for the built-in thermocouple The current measured value is shown on the left of the menu area. The calibration parameter value (in the range 1 to 12000) is shown on the right
T/C LOW		
<Slot1 name> HIGH	<i>Note 1</i>	Dual low and high point calibration parameters for the module in Slot 1. The current measured value is shown on the left of the menu area. The calibration parameter value (in the range 1 to 12000) is shown on the right
<Slot1 name> LOW		
<Slot2 name> HIGH	<i>Note 2</i>	Dual low and high point calibration parameters for the module in Slot 2 The current measured value is shown on the left of the menu area. The calibration parameter value (in the range 1 to 12000) is shown on the right
<Slot2 name> LOW		
AO1 Calibrate High		Analogue 1 Output high point calibration. This should be adjusted whilst measuring the voltage on analogue 1. Range ± 500 .
AO2 Calibrate High		Analogue 2 Output high point calibration. This should be adjusted whilst measuring the voltage on analogue 2. Range ± 500 .

Note 1: Only if module installed in Slot 1

13 Setup Menu and Miscellaneous Parameters

The Setup menu provides control over a range of miscellaneous controller-wide parameters, such as component naming, communications, display pressure units, menu and display operation, as well as several operational parameters.

13.1 Component Naming

For identification purposes, the ion gauge(s) and secondary gauges can be given 3 character names which are displayed with the corresponding pressure. In addition, each controller can be given a unique 3 character name, for example, to aid identification over comms.

The names can be made up of any combination of the following characters: <space>, '0' to '9', 'A' to 'Z' and 'a' to 'z'. As

for numerical data input, each character can be changed using the **UP** and **DOWN** buttons to scroll and change the characters.

Unit Name		3 character name for the controller. <i>[The factory default is PVC]</i>
IG1 Name		3 character name for ion gauge 1
IG2 Name	<i>Note 1</i>	3 character name for ion gauge 2
Module 1 Name		3 character name for module 1
Module 2 Name		3 character name for module 2

Note 1: PVCduo only

13.2 Pressure Units

Pressures are displayed in units of mbar, Torr or Pascal. Notes:

- Trip settings are interpreted numerically in the currently selected units
- Ion gauges can individually be selected to display as ion current (Amps) rather than in pressure units.

Pressure Units	mBar Torr Pascal
-----------------------	--

13.3 Menu and Display Related Parameters

Menu Escape Time	If in Menu or Parameter Edit modes, and no button press is executed, the controller will automatically revert to the last viewed Status page after waiting for the Menu Escape Time . Range: 20 to 999 seconds
Display Saver	Turns display saver functionality on and off
Display Saver Time	If turned on, the time between the last button press and the start of screen display. Range: 1 to 999 minutes
Bar Graph Minimum	For the BarGraph page, the minimum exponent value. For example, a value of -12 equates to 10^{-12} .
Bar Graph Maximum	For the BarGraph page, the maximum exponent value. For example, a value of -3 equates to 10^{-3} .

13.4 Communications Parameters

The PVC provide extensive support for control and monitoring over serial RS232 and RS485:

Comms Address	Each controller on a serial bus must have a unique address set in this parameter. Range: 01 to 99
Comms Protocol	Communications can be executed using either a binary MODBUS-based RTE protocol, or via an ASCII-based protocol: MODBUS LITend : MODBUS RTE using little endian data transfer MODBUS BIGend : MODBUS RTE using big endian data transfer QueBUS-No Check : QueBus ASCII protocol without error checking QueBUS+CS : QueBus ASCII protocol with simple check sum error checking QueBUS+CRC : QueBus ASCII protocol with full Cyclical Redundancy Check
Comms Baud Rate	4800 , 9600 , 19200 , 38400 or 57600 baud
Comms Parity	None , Even or Odd
Comms Indicator	Turns the comms indicator on and off.

13.5 Information Parameters

All information parameters are non-editable and are "locked".

Software Version	As well as the UNIT id comms parameter, to help distinguish the PVCuni and PVCduo, version numbers start at 3.00. Note that the PVCuni and PVCduo controllers use the same software – functionality is auto-detected on power up.
Heatsink Temperature	The temperature of the heatsink is monitored and controls the fan
Internal Temperature	(Diagnostics)
Int Ctrl Power	(Diagnostics)
Unit Run Time	The total operating time of the controller since last factory reset

